


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021517\
 Data File : BF092975.D
 Acq On : 16 Feb 2017 4:10
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 13 18:04:38 2017

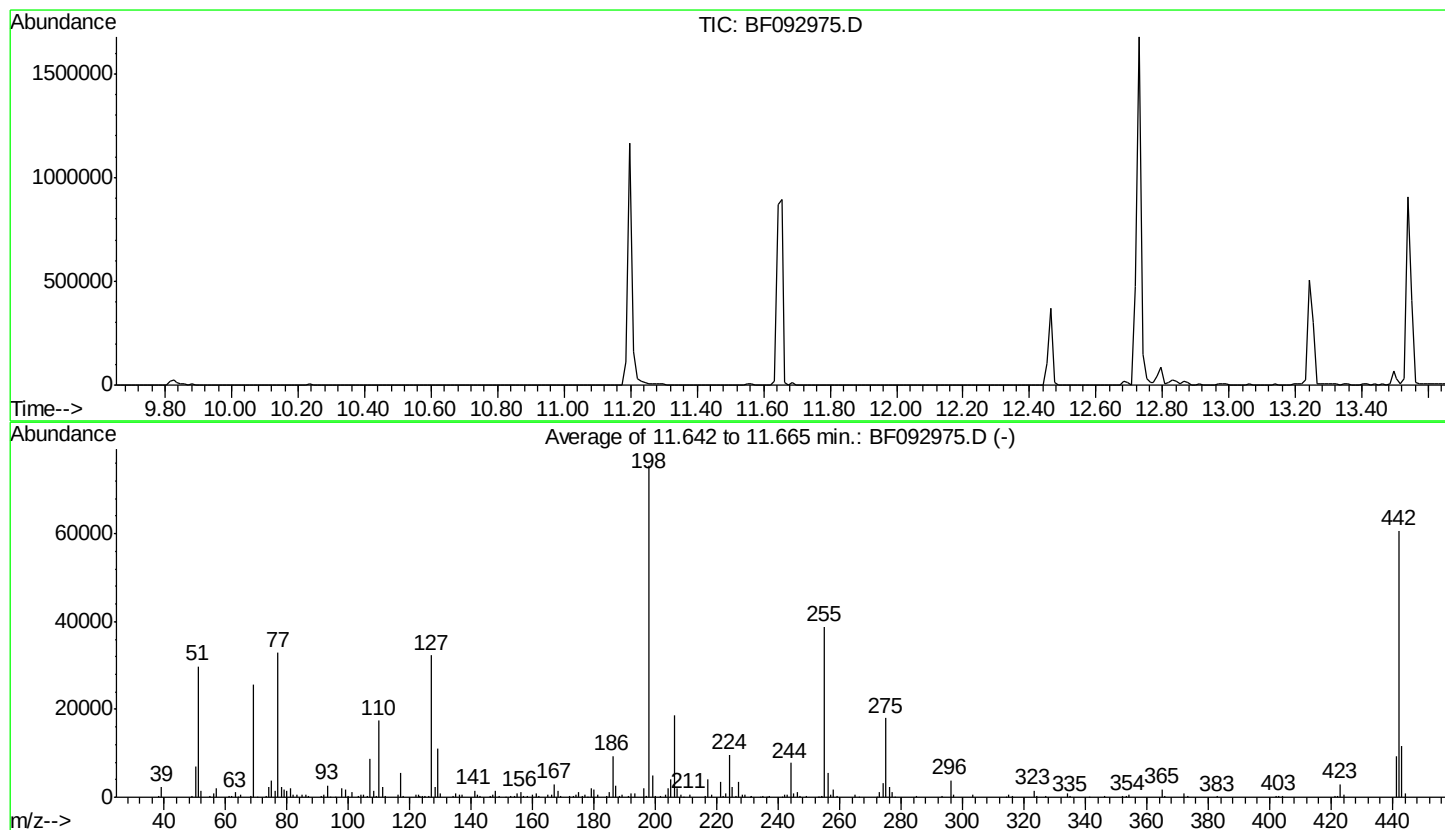

AutoFind: Scans 836, 837, 838; Background Corrected with Scan 832

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	29752	PASS
68	69	0.00	2	1.4	367	PASS
69	198	0.00	100	34.0	25674	PASS
70	69	0.00	2	0.4	111	PASS
127	198	10	80	42.7	32237	PASS
197	198	0.00	2	0.5	384	PASS
198	198	100	100	100.0	75520	PASS
199	198	5	9	6.4	4838	PASS
275	198	10	60	23.8	17968	PASS
365	198	1	100	2.4	1792	PASS
441	442	0.01	24	15.5	9411	PASS
442	198	50	100	80.3	60671	PASS
443	442	15	24	19.0	11542	PASS