
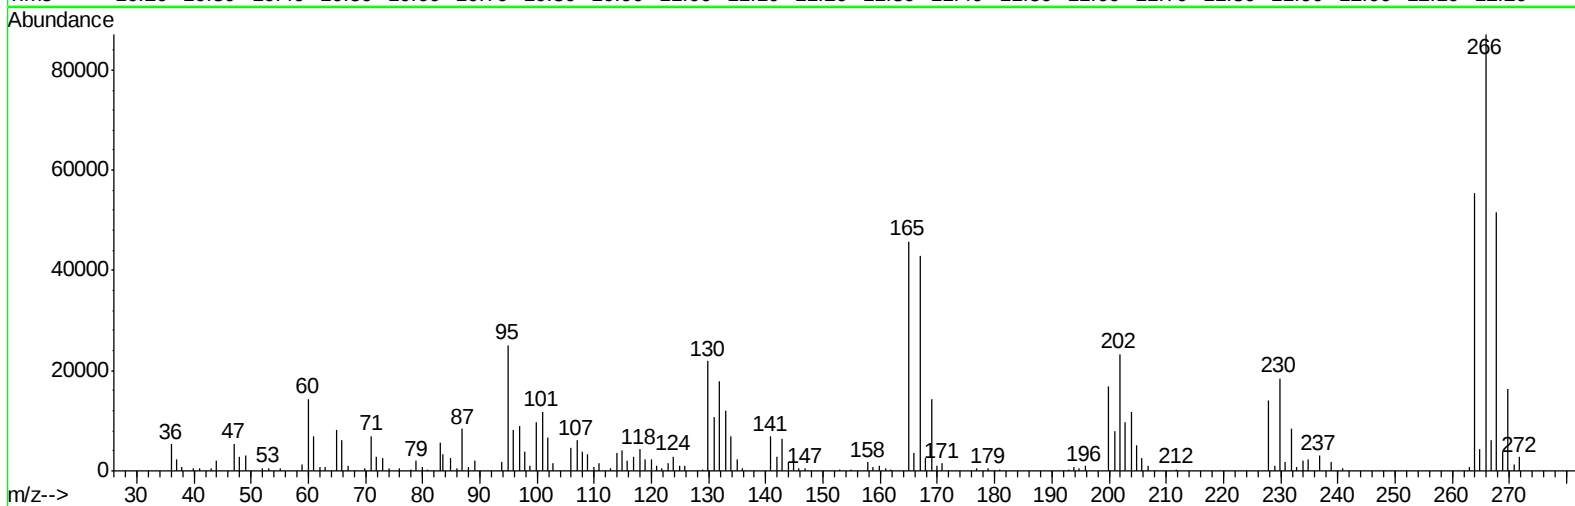


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021518\
Data File : BF103009.D
Acq On : 15 Feb 2018 10:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 05:10:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 14:08:58 2018
Response via : Initial Calibration

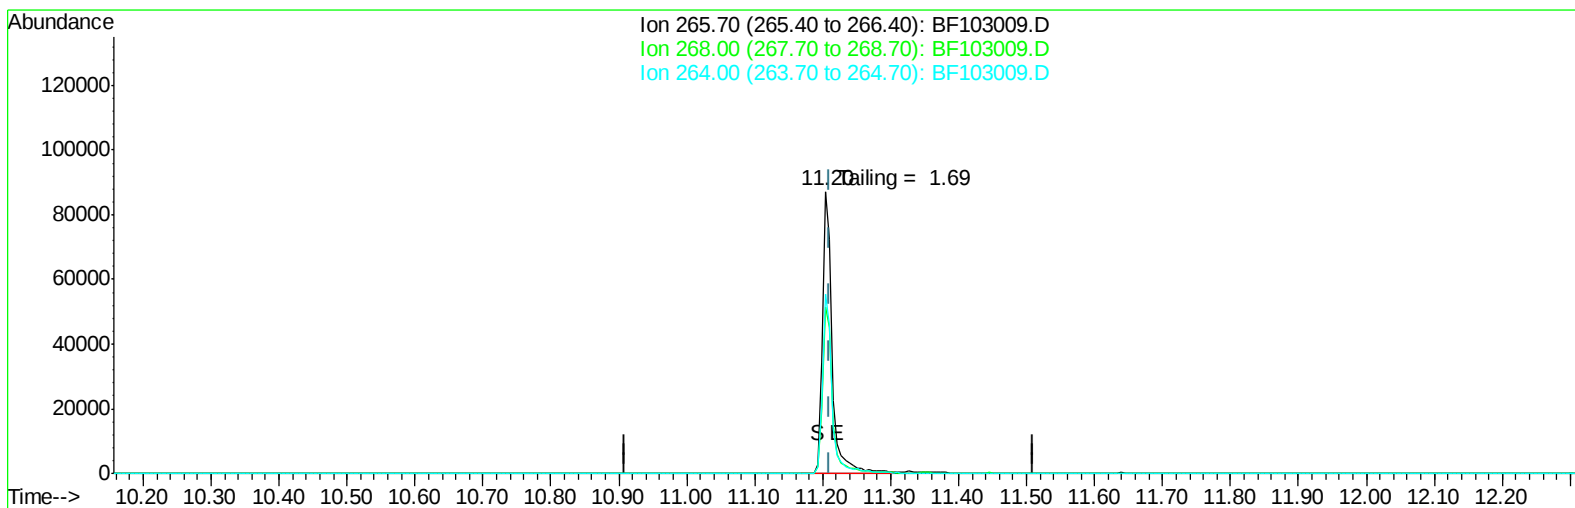

TIC: BF103009.D

(69) Pentachlorophenol (C)



11.204min (-0.006) 45705.60ng

response 89546

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	59.10
264.00	61.90	63.52
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021518\
Data File : BF103009.D
Acq On : 15 Feb 2018 10:40
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 16 05:10:33 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 15 14:08:58 2018
Response via : Initial Calibration

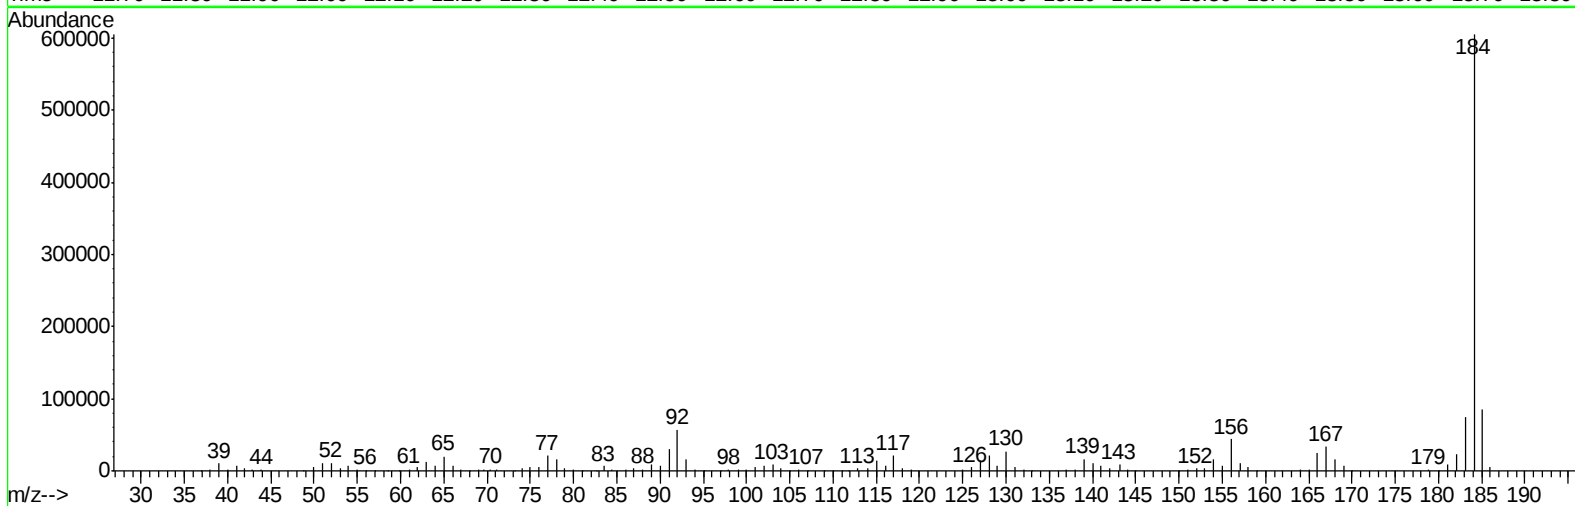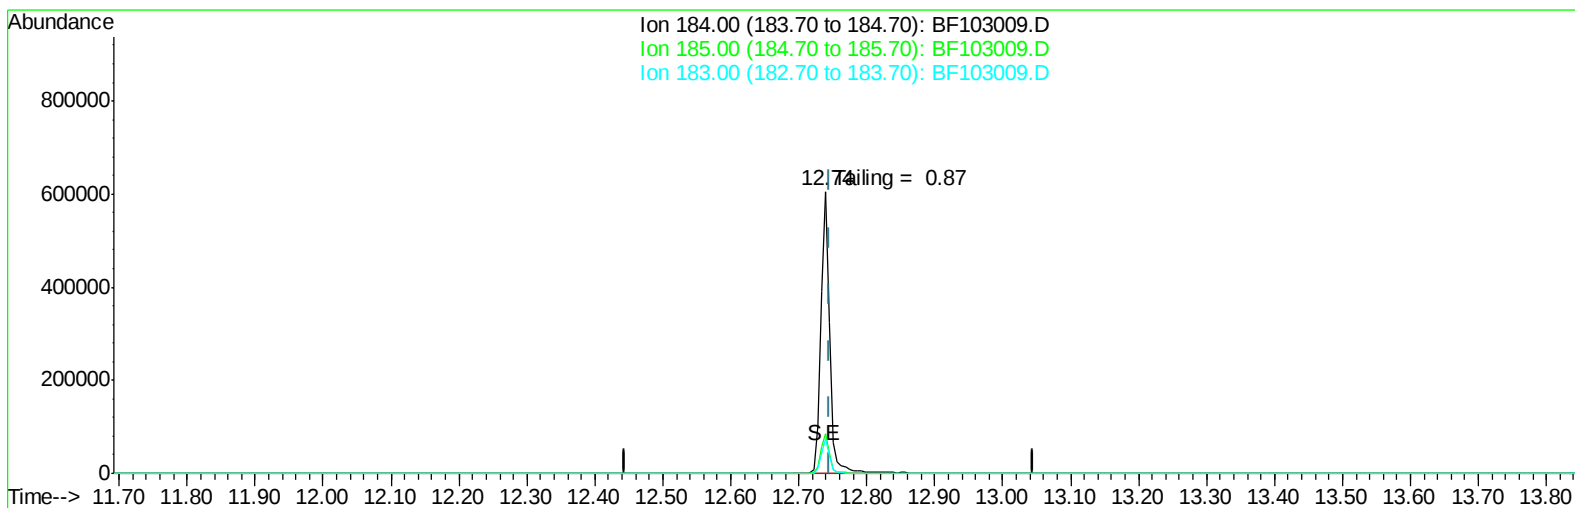

TIC: BF103009.D

(76) Benzidine

12.739min (-0.006) 0.00ng

response 563611

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.17
183.00	11.60	12.21
0.00	0.00	0.00