


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF021518\
 Data File : BF103009.D
 Acq On : 15 Feb 2018 10:40
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 15 14:08:58 2018

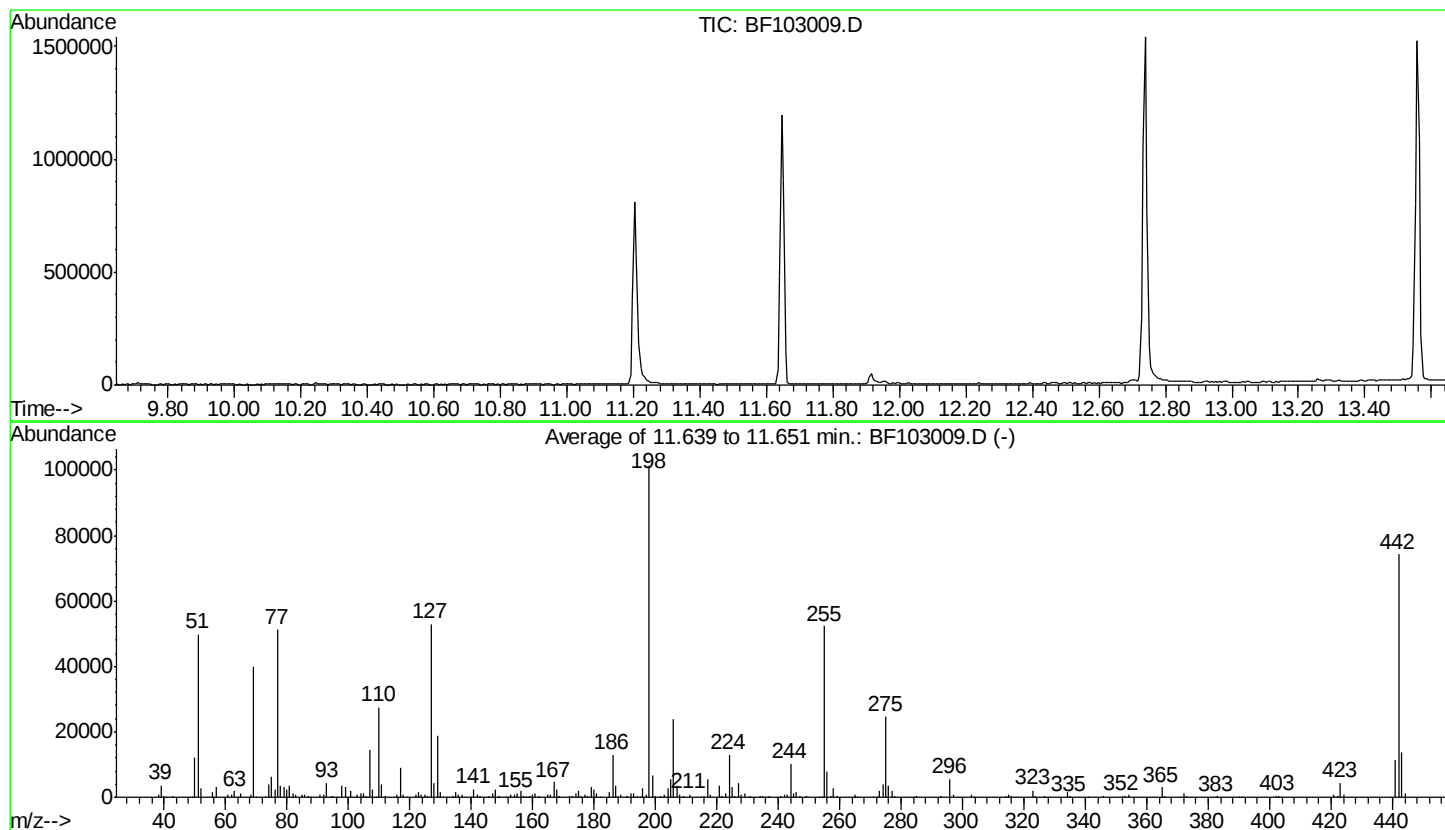

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	49.2	49872	PASS
68	69	0.00	2	1.9	750	PASS
69	198	0.00	100	39.2	39737	PASS
70	69	0.00	2	0.5	180	PASS
127	198	10	80	52.1	52842	PASS
197	198	0.00	2	0.8	766	PASS
198	198	100	100	100.0	101352	PASS
199	198	5	9	6.4	6483	PASS
275	198	10	60	24.3	24648	PASS
365	198	1	100	3.0	3039	PASS
441	443	0.01	100	83.4	11539	PASS
442	198	50	100	73.2	74210	PASS
443	442	15	24	18.6	13839	PASS