


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF021518\
Data File : BF103035.D
Acq On : 15 Feb 2018 23:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 15 14:08:58 2018

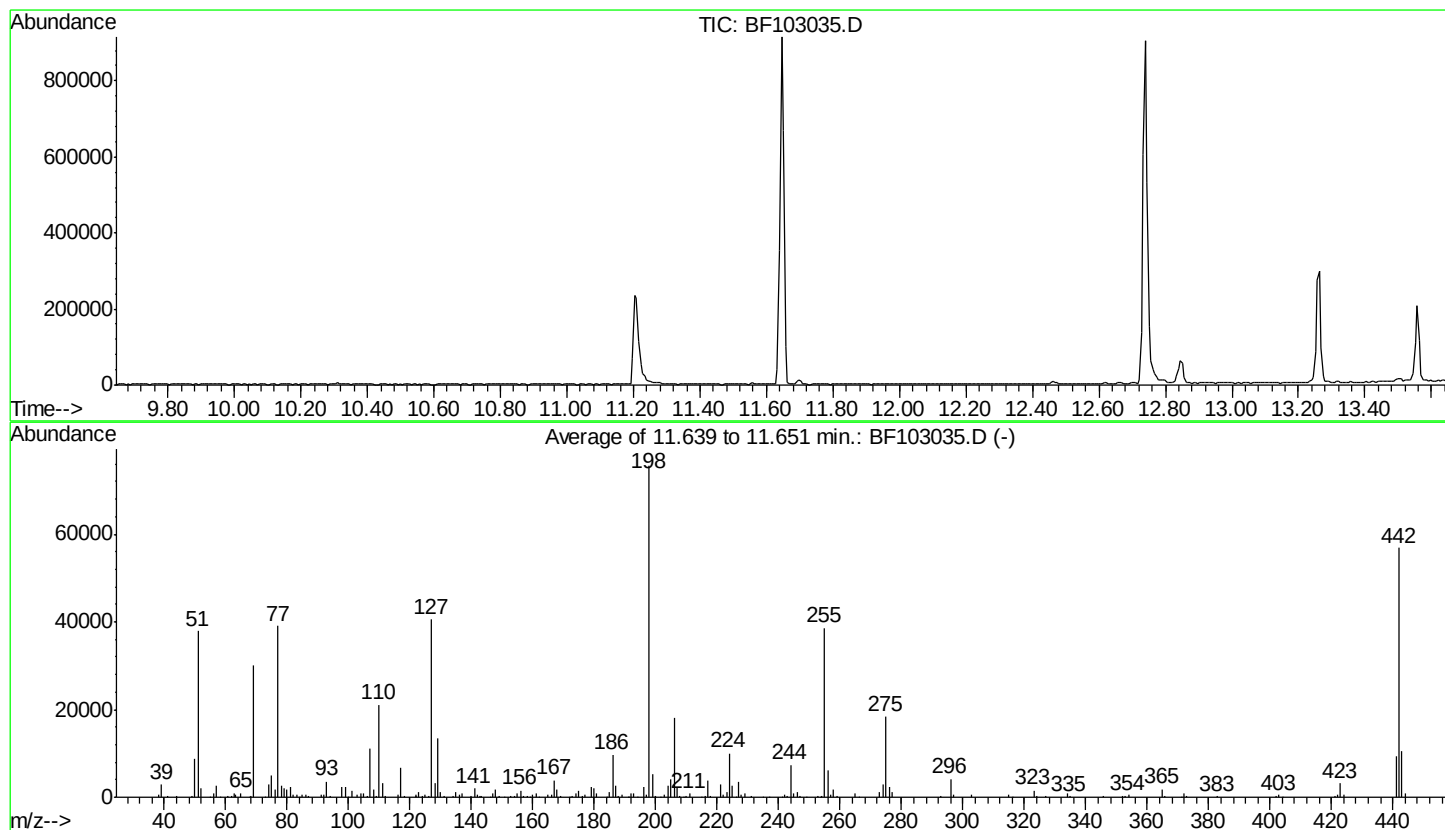

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.1	37859	PASS
68	69	0.00	2	1.0	288	PASS
69	198	0.00	100	39.8	30104	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.5	40496	PASS
197	198	0.00	2	0.7	511	PASS
198	198	100	100	100.0	75632	PASS
199	198	5	9	6.9	5238	PASS
275	198	10	60	24.3	18353	PASS
365	198	1	100	2.4	1801	PASS
441	443	0.01	100	87.0	9235	PASS
442	198	50	100	75.2	56907	PASS
443	442	15	24	18.7	10618	PASS