
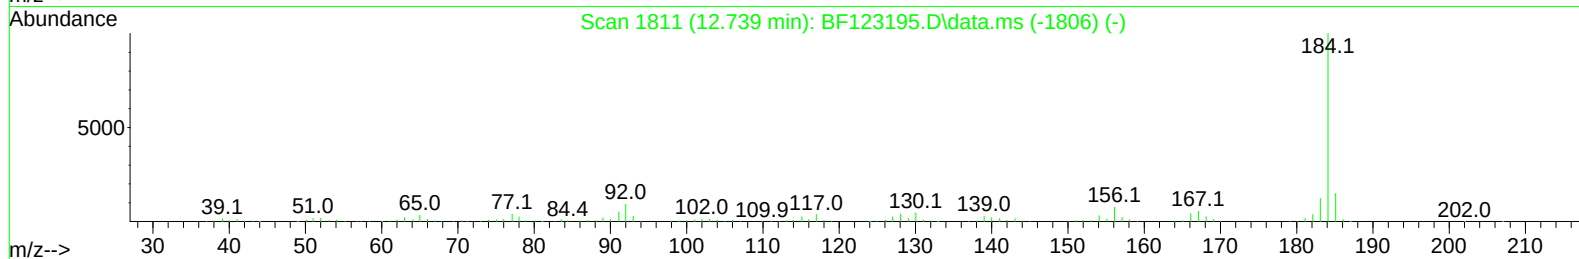
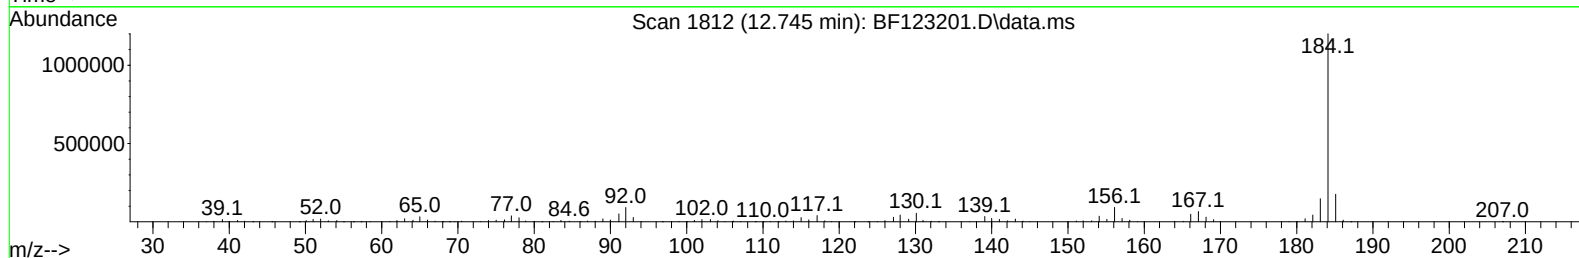


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021521\
Data File : BF123201.D
Acq On : 15 Feb 2021 12:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 13:43:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

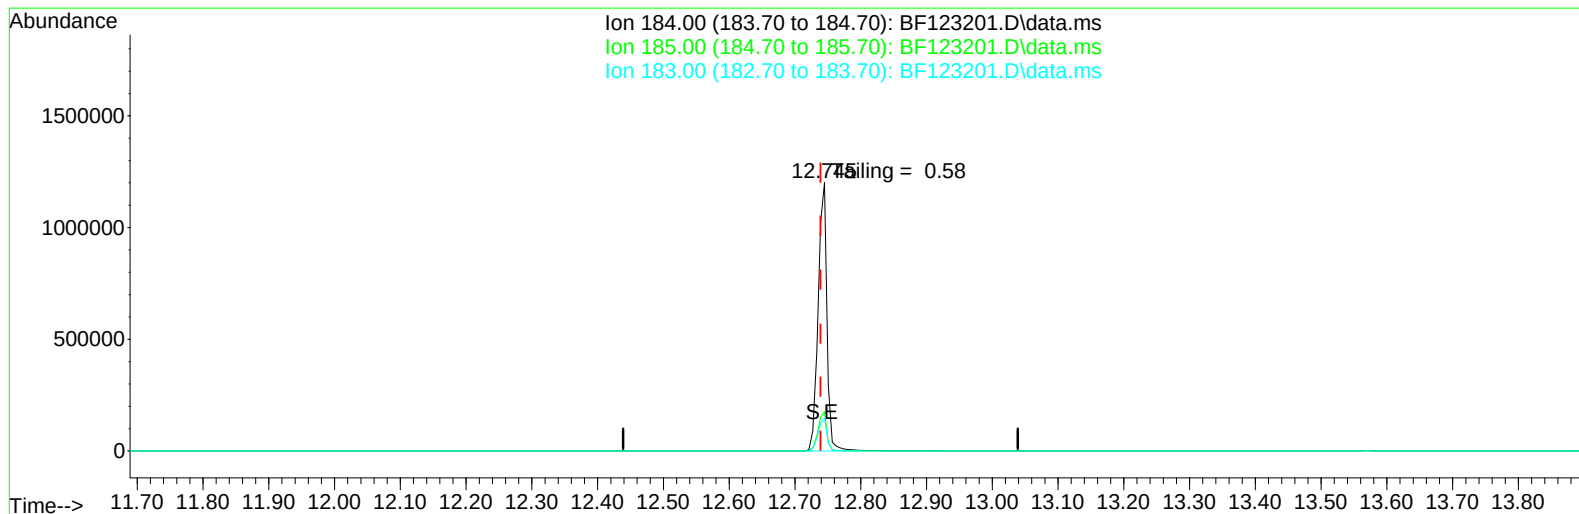

TIC: BF123201.D\data.ms

(77) Benzidine




12.745min (+ 0.006) 0.00 ng

response 1123577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.63
183.00	12.10	12.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021521\
Data File : BF123201.D
Acq On : 15 Feb 2021 12:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 15 13:43:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

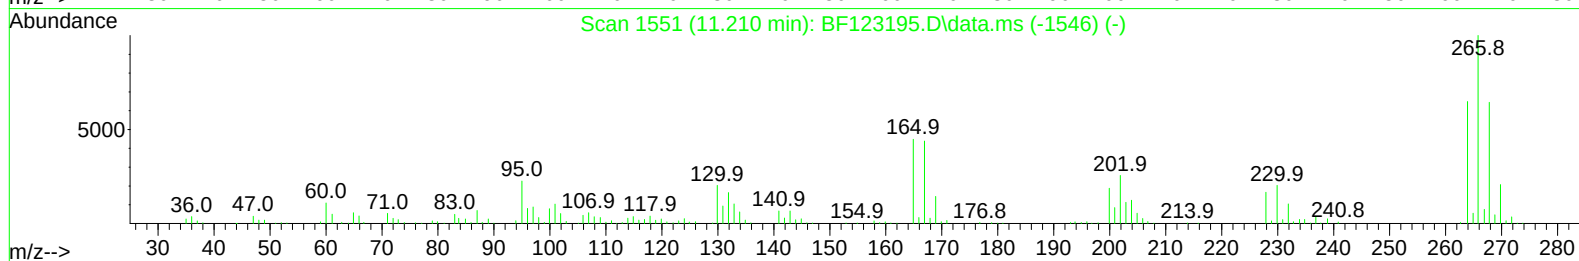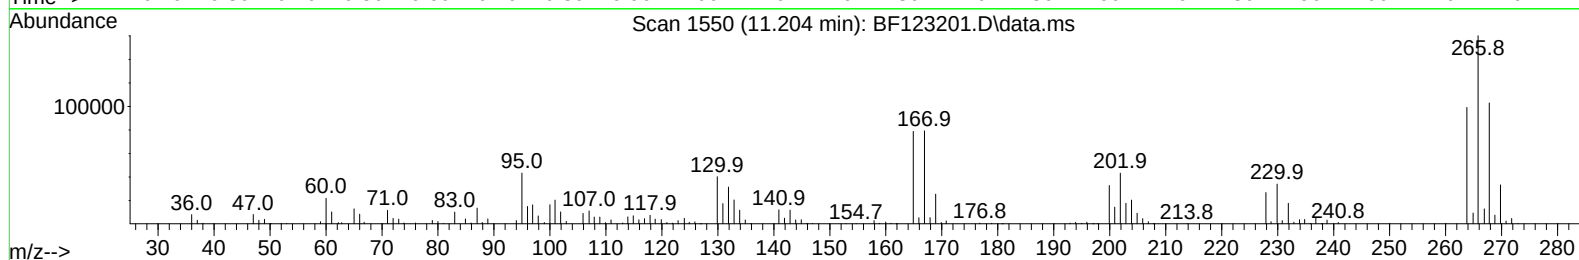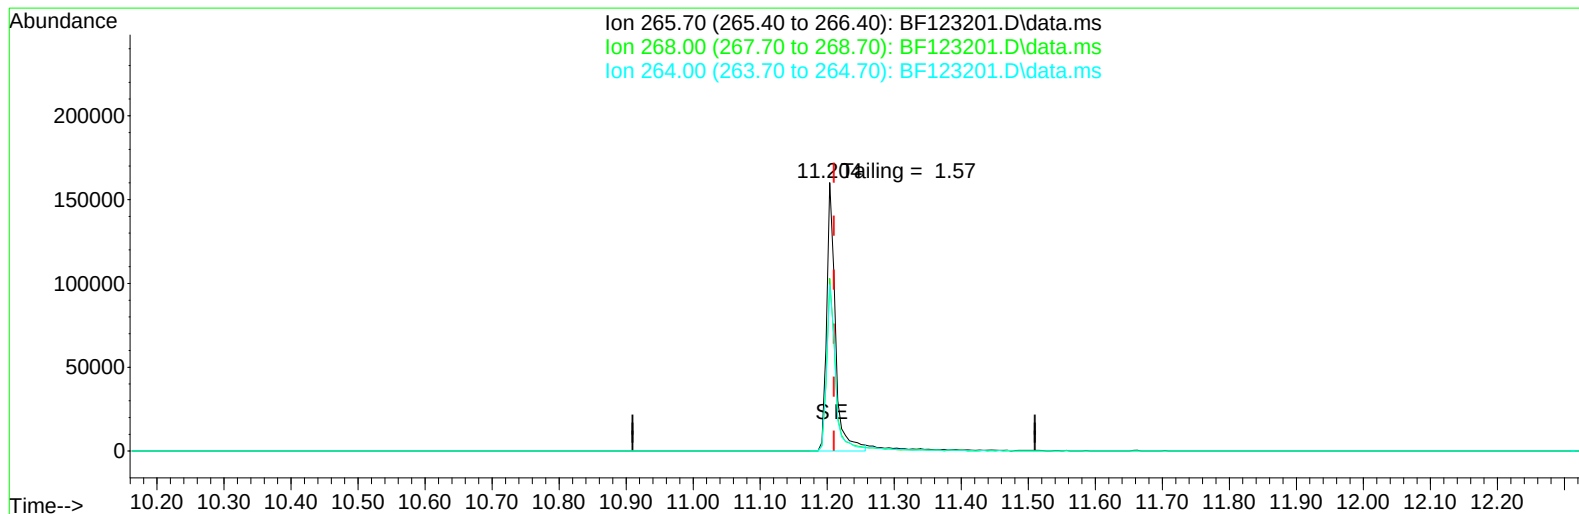

TIC: BF123201.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 38409.55 ng

response 151946

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.30
264.00	62.30	61.98
0.00	0.00	0.00