
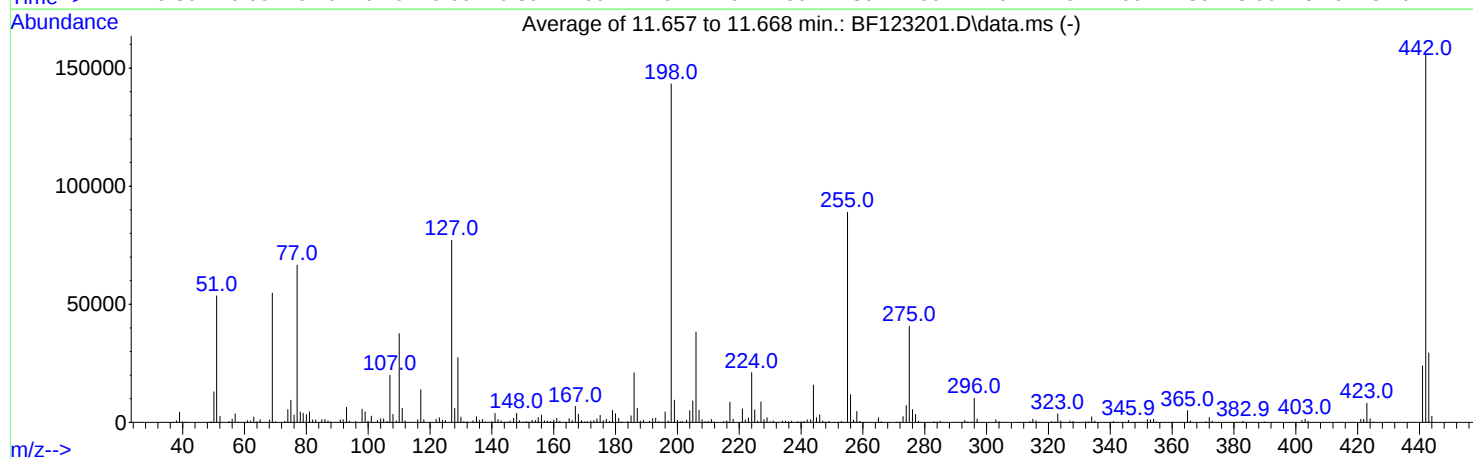


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021521\
 Data File : BF123201.D
 Acq On : 15 Feb 2021 12:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 12 16:59:49 2021

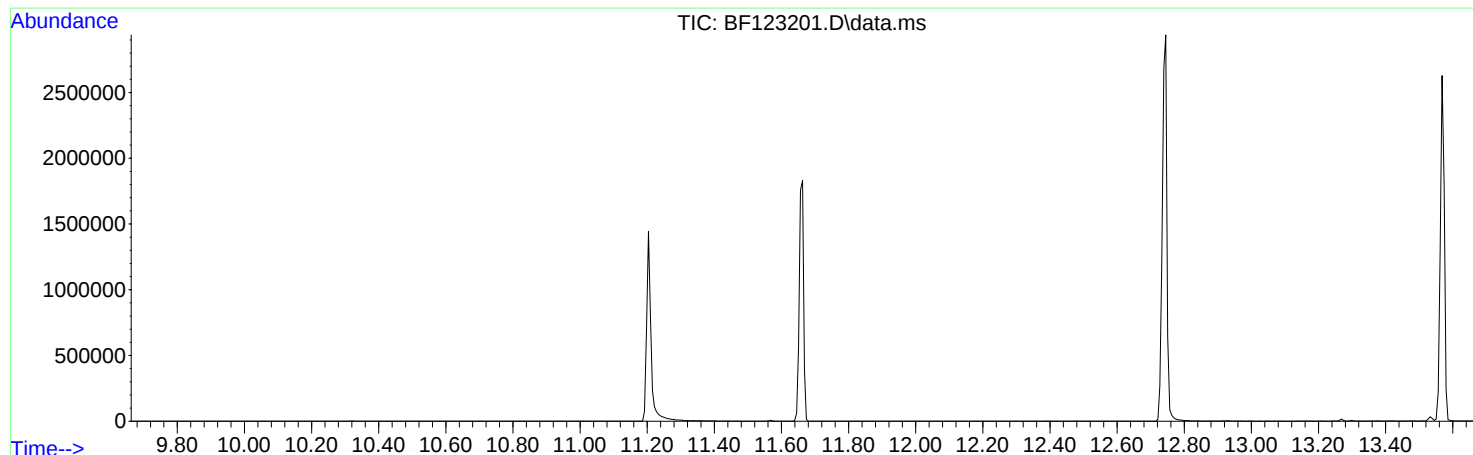




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.4	53581	PASS
68	69	0.00	2	1.8	1007	PASS
69	198	0.00	100	38.2	54768	PASS
70	69	0.00	2	0.5	252	PASS
127	198	10	80	53.8	77104	PASS
197	198	0.00	2	0.5	670	PASS
198	198	100	100	100.0	143307	PASS
199	198	5	9	6.6	9408	PASS
275	198	10	60	28.4	40656	PASS
365	198	1	100	3.4	4923	PASS
441	198	0.01	100	16.7	23898	PASS
442	442	50	100	100.0	155755	PASS
443	442	15	24	18.9	29421	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021521\
 Data File : BF123201.D
 Acq On : 15 Feb 2021 12:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 15 13:43:46 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 12 16:59:49 2021
 Response via : Initial Calibration

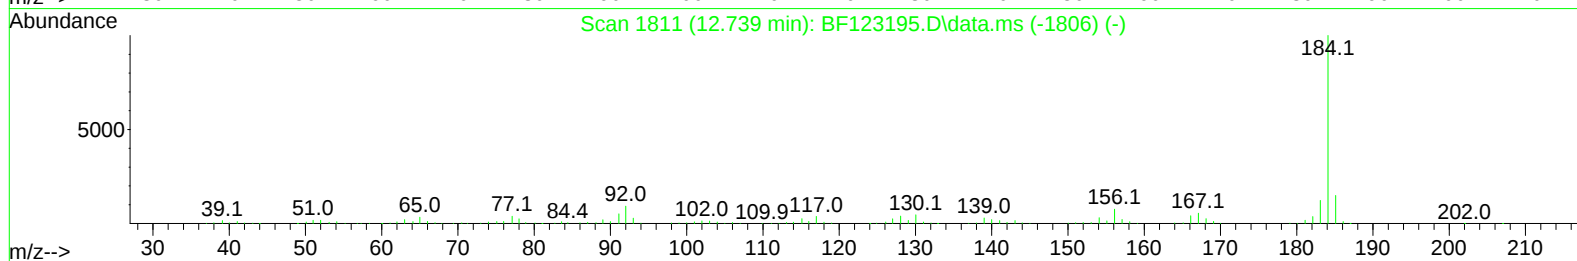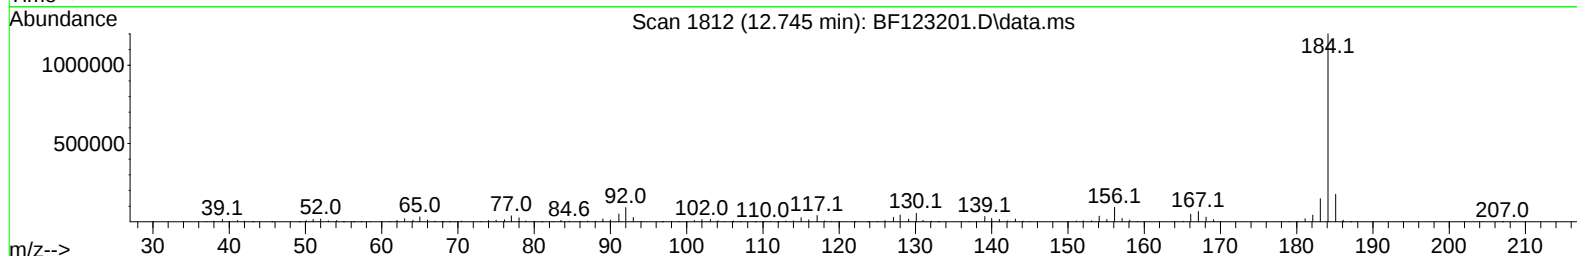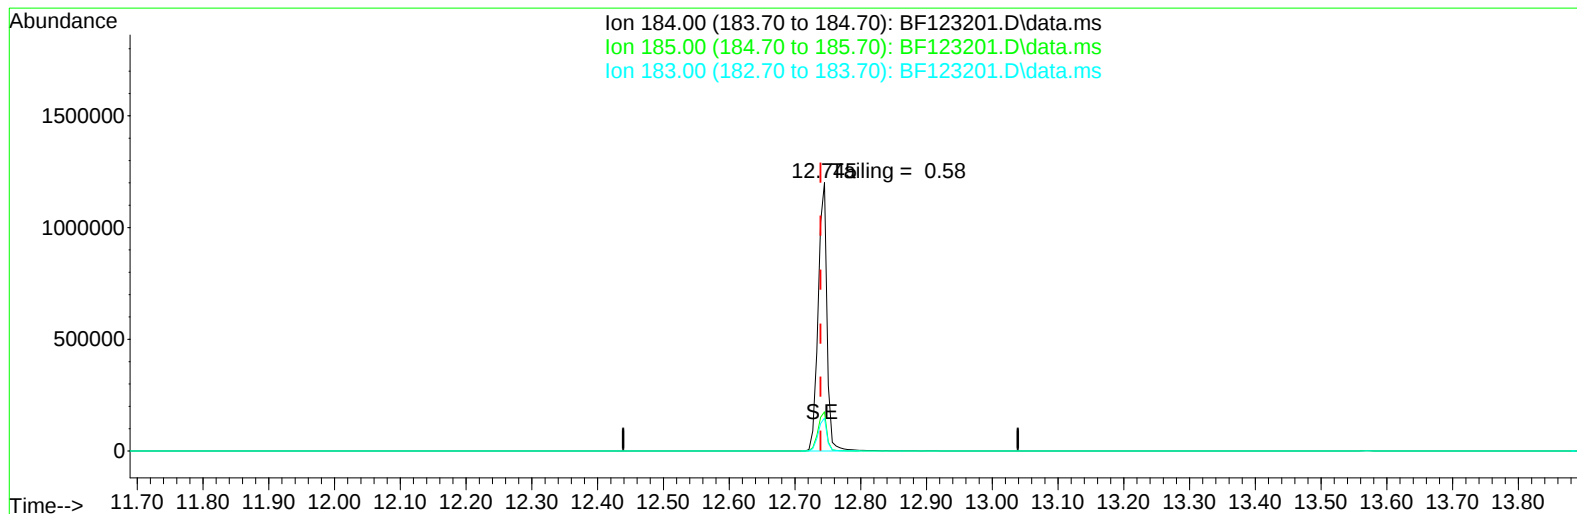

TIC: BF123201.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng




response 1123577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.63
183.00	12.10	12.32
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021521\  
Data File : BF123201.D  
Acq On    : 15 Feb 2021  12:38  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 15 13:43:46 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

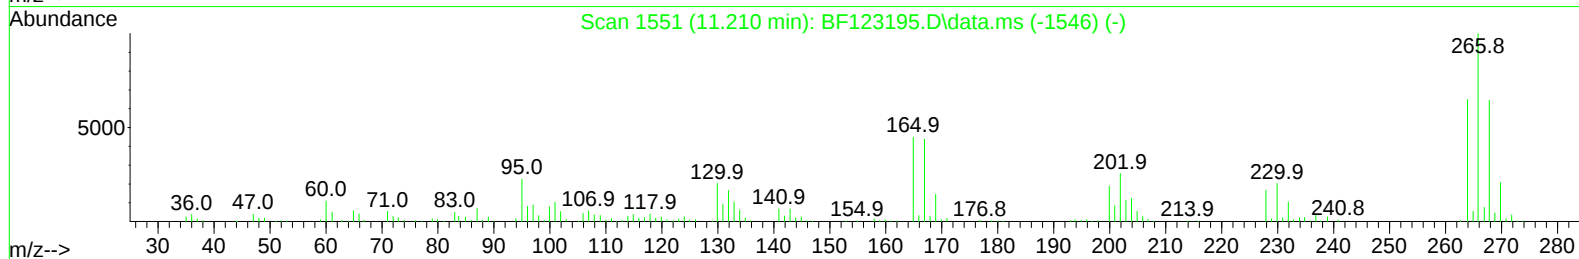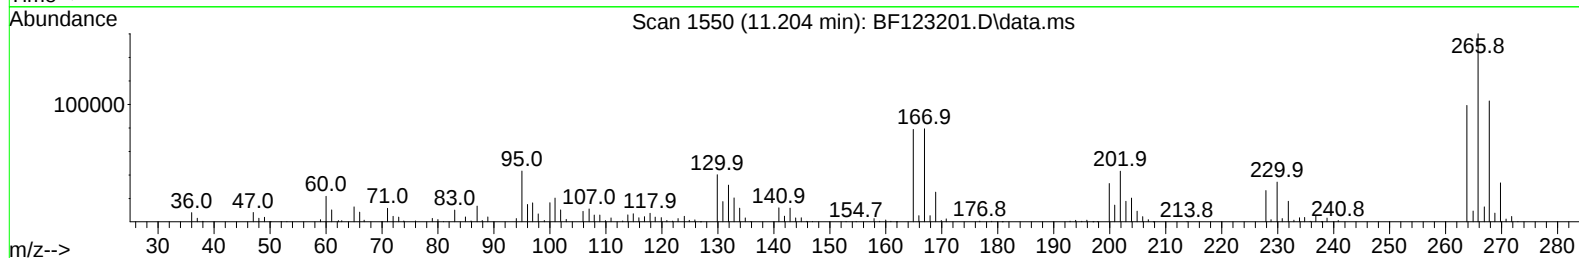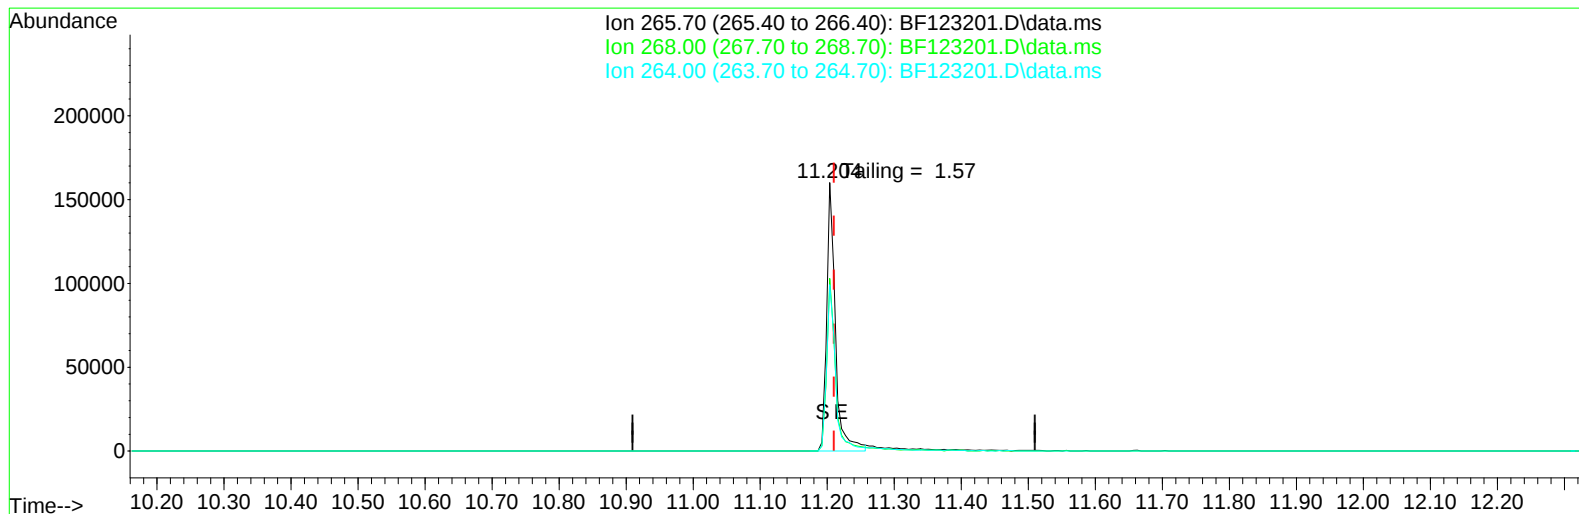

TIC: BF123201.D\data.ms

(70) Pentachlorophenol (C)

11.204min (-0.006) 38409.55 ng

response **151946**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	64.30
264.00	62.30	61.98
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
02/15/2021	BNA_F	<u>BF123201.D</u>
Compound Name	Response	Retention Time
DDT	425272	13.56
DDD	3407	13.26
DDE	784	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4191	429463	0.98

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP