

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
 Data File : BF126900.D
 Acq On : 15 Feb 2022 19:12
 Operator : CG\JU
 Sample : N1477-05
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SPLP-LEACHATE-AMENDED-COMP-7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126900.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.163	485	489	496	rVB	72489	78465	2.67%	0.502%
2	5.557	548	556	560	rBV	1517281	1389168	47.34%	8.896%
3	6.557	722	726	730	rBV	876718	806128	27.47%	5.162%
4	6.939	788	791	795	rBV	654635	509652	17.37%	3.264%
5	6.992	797	800	806	rBV	47332	44987	1.53%	0.288%
6	7.504	882	887	890	rBV	2091299	1942918	66.21%	12.442%
7	7.675	912	916	919	rVB	77225	69632	2.37%	0.446%
8	7.933	954	960	967	rVB3	39669	60059	2.05%	0.385%
9	8.116	988	991	1001	rBV	151234	139913	4.77%	0.896%
10	8.222	1006	1009	1013	rBV	754795	631082	21.50%	4.041%
11	8.433	1042	1045	1047	rBV	41942	35663	1.22%	0.228%
12	8.457	1047	1049	1054	rVB	50820	39974	1.36%	0.256%
13	9.298	1186	1192	1195	rBV	3641631	2934677	100.00%	18.792%
14	9.369	1201	1204	1206	rVB	66858	47379	1.61%	0.303%
15	9.433	1212	1215	1222	rVB	61597	66981	2.28%	0.429%
16	9.686	1255	1258	1261	rBV	70407	55553	1.89%	0.356%
17	9.775	1270	1273	1283	rBV	66063	83263	2.84%	0.533%
18	9.898	1289	1294	1297	rBV2	57557	51194	1.74%	0.328%
19	9.980	1304	1308	1311	rBV	767480	585007	19.93%	3.746%
20	10.375	1371	1375	1377	rBV	40975	44895	1.53%	0.287%
21	10.392	1377	1378	1382	rVB2	44799	38840	1.32%	0.249%
22	10.769	1438	1442	1446	rBV	1806596	1624500	55.36%	10.403%
23	10.874	1458	1460	1465	rVB2	35654	39835	1.36%	0.255%
24	11.321	1533	1536	1539	rBV	39442	38503	1.31%	0.247%
25	11.416	1547	1552	1555	rBV	61908	54676	1.86%	0.350%
26	11.469	1558	1561	1565	rBV	583747	520734	17.74%	3.335%
27	11.980	1645	1648	1651	rBV	95549	86366	2.94%	0.553%
28	13.057	1827	1831	1834	rBV	2735523	2408345	82.07%	15.422%
29	13.945	1978	1982	1995	rBV	264181	363697	12.39%	2.329%
30	14.115	2007	2011	2015	rBV	494392	435164	14.83%	2.787%
31	14.739	2114	2117	2120	rVB2	38087	37774	1.29%	0.242%
32	15.627	2263	2268	2273	rBV	281871	351373	11.97%	2.250%




Sum of corrected areas: 15616397

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
Data File : BF126900.D
Acq On : 15 Feb 2022 19:12
Operator : CG\JU
Sample : N1477-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

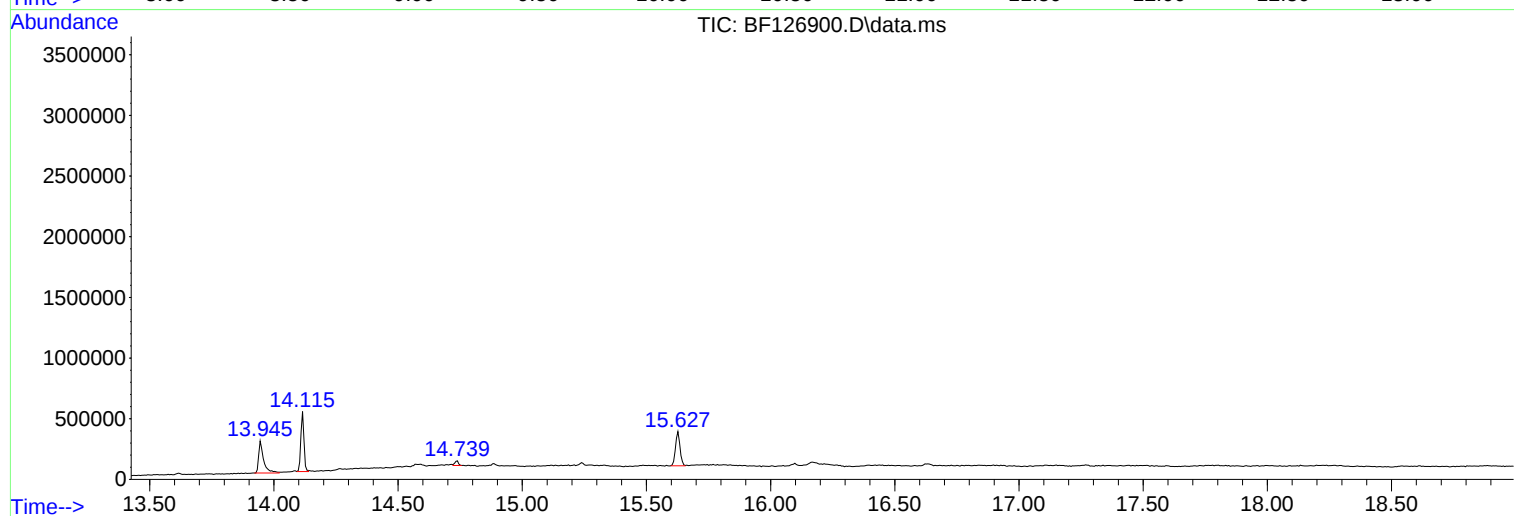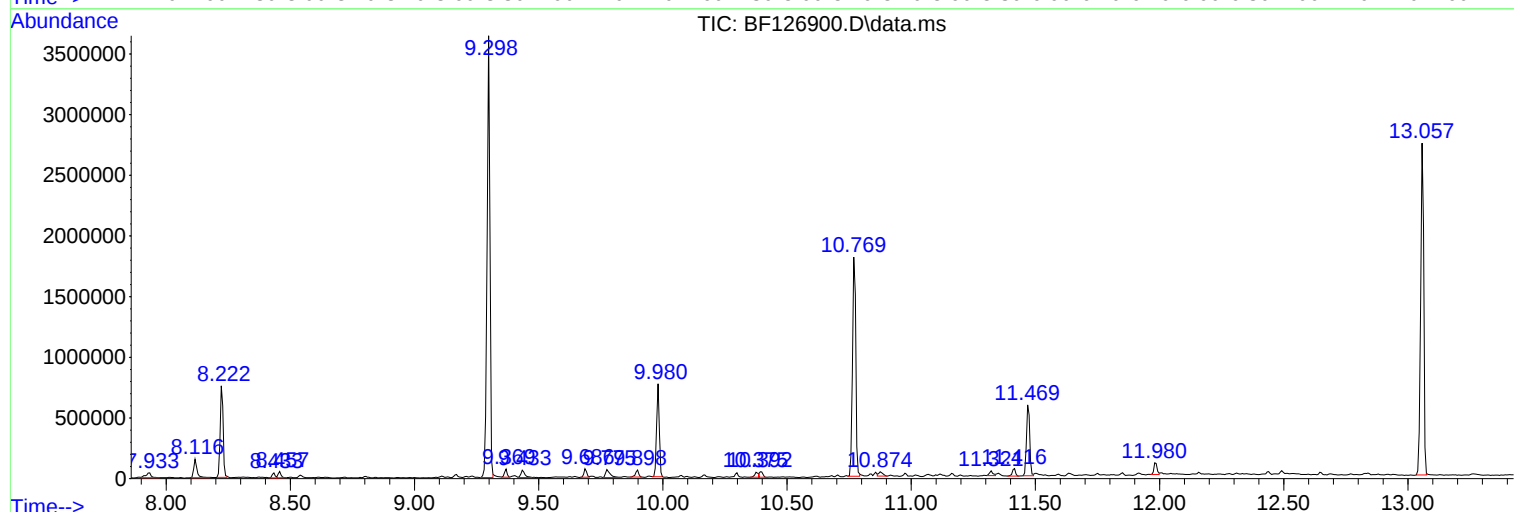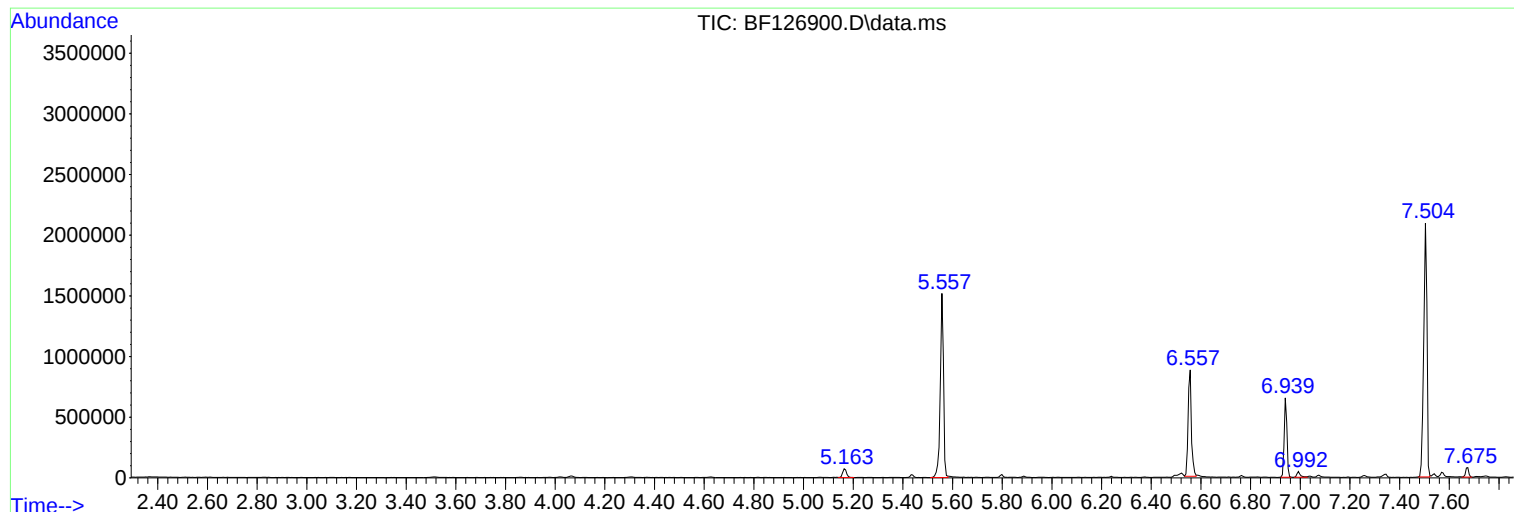

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
Data File : BF126900.D
Acq On : 15 Feb 2022 19:12
Operator : CG\JU
Sample : N1477-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
Data File : BF126900.D
Acq On : 15 Feb 2022 19:12
Operator : CG\JU
Sample : N1477-05
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SPLP-LEACHATE-AMENDED-COMP-7

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------