

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021522\  
 Data File : BF126901.D  
 Acq On : 15 Feb 2022 19:40  
 Operator : CG\JU  
 Sample : N1477-06  
 Misc :  
 ALS Vial : 19 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 SPLP-LEACHATE-AMENDED-COMP-8

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126901.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.163       | 485           | 489         | 496          | rVB      | 65931          | 75433         | 2.24%           | 0.434%        |
| 2         | 5.557       | 552           | 556         | 559          | rBV      | 1707034        | 1460405       | 43.43%          | 8.407%        |
| 3         | 6.557       | 722           | 726         | 731          | rBV      | 1047034        | 950988        | 28.28%          | 5.475%        |
| 4         | 6.940       | 788           | 791         | 795          | rBV      | 820631         | 655257        | 19.49%          | 3.772%        |
| 5         | 6.993       | 797           | 800         | 804          | rBV      | 47508          | 39165         | 1.16%           | 0.225%        |
| 6         | 7.504       | 882           | 887         | 890          | rBV      | 2253013        | 2201265       | 65.46%          | 12.672%       |
| 7         | 8.116       | 988           | 991         | 1000         | rBV      | 110029         | 102042        | 3.03%           | 0.587%        |
| 8         | 8.222       | 1006          | 1009        | 1013         | rBV      | 978238         | 811253        | 24.13%          | 4.670%        |
| 9         | 8.434       | 1042          | 1045        | 1047         | rBV      | 57107          | 45144         | 1.34%           | 0.260%        |
| 10        | 8.457       | 1047          | 1049        | 1054         | rVB      | 71319          | 53752         | 1.60%           | 0.309%        |
| 11        | 9.298       | 1188          | 1192        | 1195         | rBV      | 4059835        | 3362546       | 100.00%         | 19.357%       |
| 12        | 9.434       | 1212          | 1215        | 1225         | rVB      | 48654          | 56132         | 1.67%           | 0.323%        |
| 13        | 9.775       | 1270          | 1273        | 1280         | rBV2     | 36756          | 46701         | 1.39%           | 0.269%        |
| 14        | 9.898       | 1290          | 1294        | 1299         | rVB      | 44929          | 43745         | 1.30%           | 0.252%        |
| 15        | 9.981       | 1304          | 1308        | 1311         | rBV      | 965013         | 761133        | 22.64%          | 4.382%        |
| 16        | 10.769      | 1438          | 1442        | 1446         | rBV      | 2044718        | 1877097       | 55.82%          | 10.806%       |
| 17        | 11.469      | 1558          | 1561        | 1565         | rBV      | 752779         | 681992        | 20.28%          | 3.926%        |
| 18        | 11.980      | 1645          | 1648        | 1652         | rBV      | 64625          | 57453         | 1.71%           | 0.331%        |
| 19        | 13.057      | 1827          | 1831        | 1835         | rBV      | 2896031        | 2855490       | 84.92%          | 16.438%       |
| 20        | 13.945      | 1979          | 1982        | 1991         | rBV      | 156535         | 222202        | 6.61%           | 1.279%        |
| 21        | 14.116      | 2007          | 2011        | 2017         | rVB      | 656850         | 561923        | 16.71%          | 3.235%        |
| 22        | 15.627      | 2263          | 2268        | 2275         | rBV      | 351571         | 449830        | 13.38%          | 2.590%        |




Sum of corrected areas: 17370948

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021522\  
Data File : BF126901.D  
Acq On : 15 Feb 2022 19:40  
Operator : CG\JU  
Sample : N1477-06  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPLP-LEACHATE-AMENDED-COMP-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

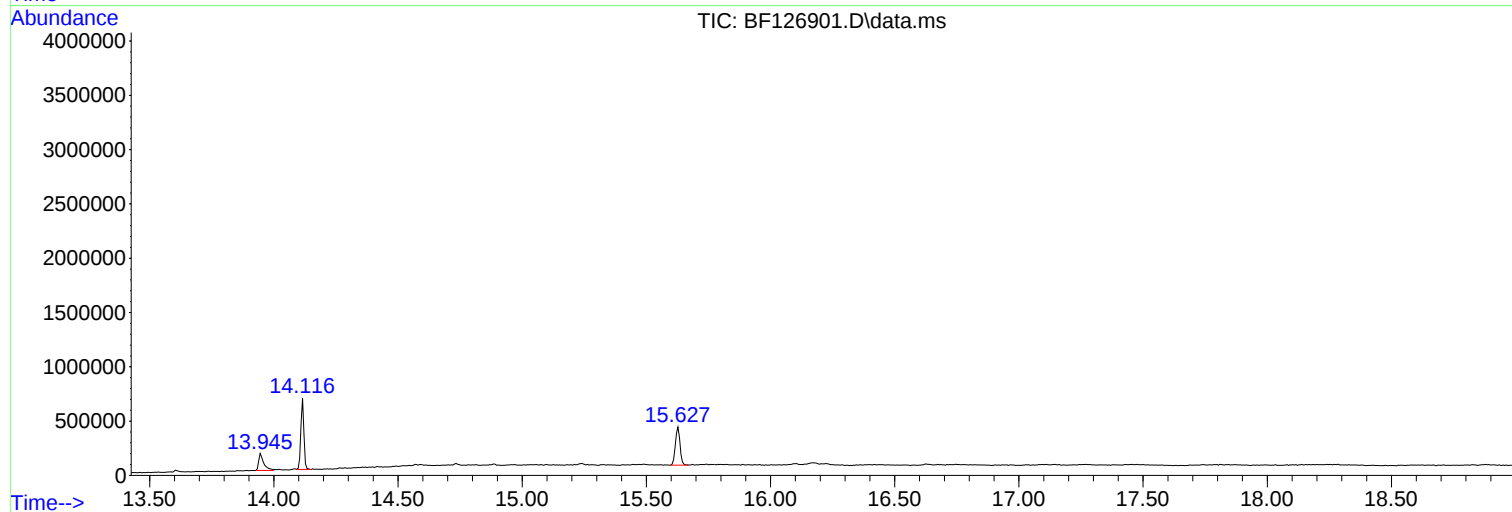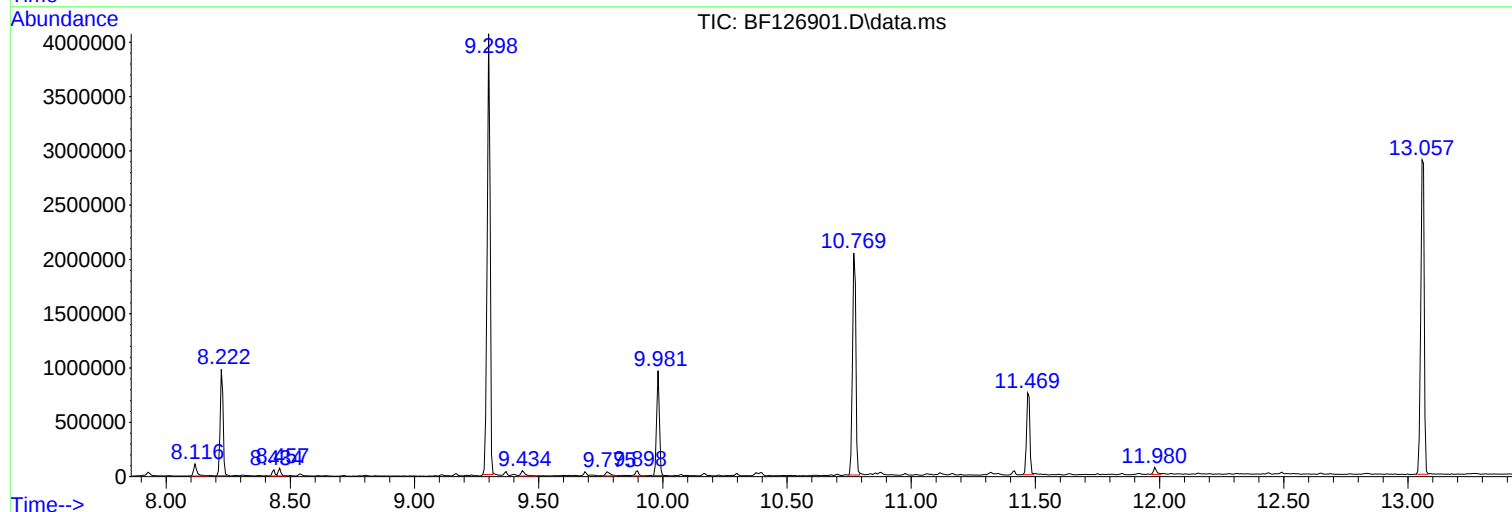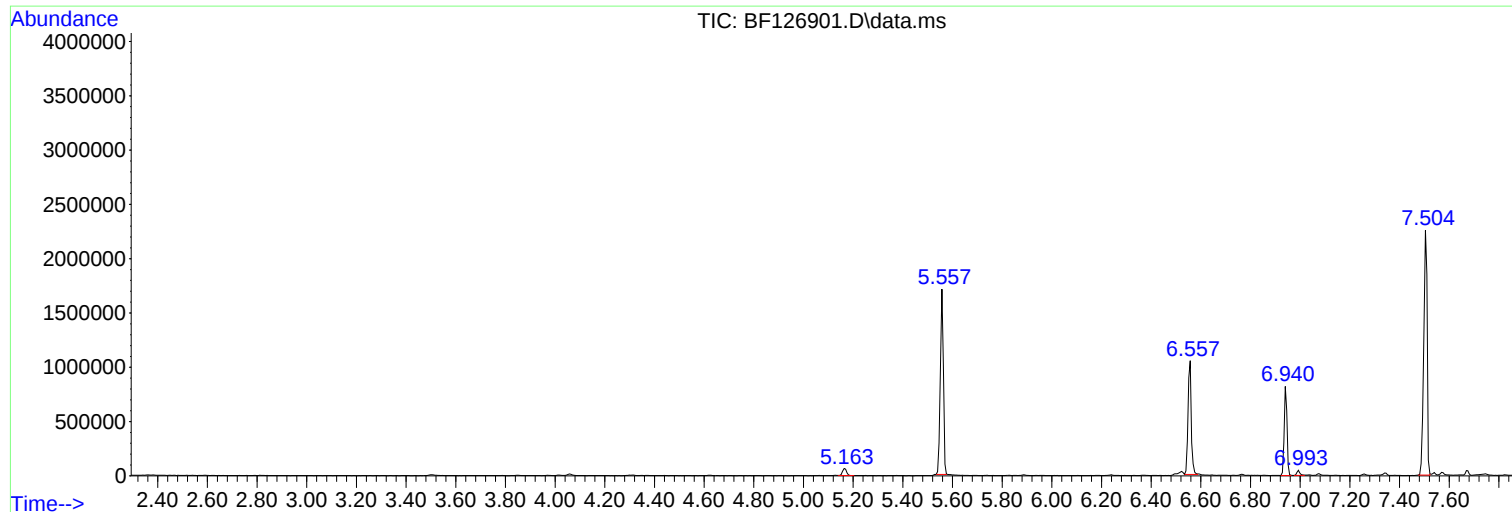

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021522\  
Data File : BF126901.D  
Acq On : 15 Feb 2022 19:40  
Operator : CG\JU  
Sample : N1477-06  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPLP-LEACHATE-AMENDED-COMP-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021522\  
Data File : BF126901.D  
Acq On : 15 Feb 2022 19:40  
Operator : CG\JU  
Sample : N1477-06  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
SPLP-LEACHATE-AMENDED-COMP-8

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF020922.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|