
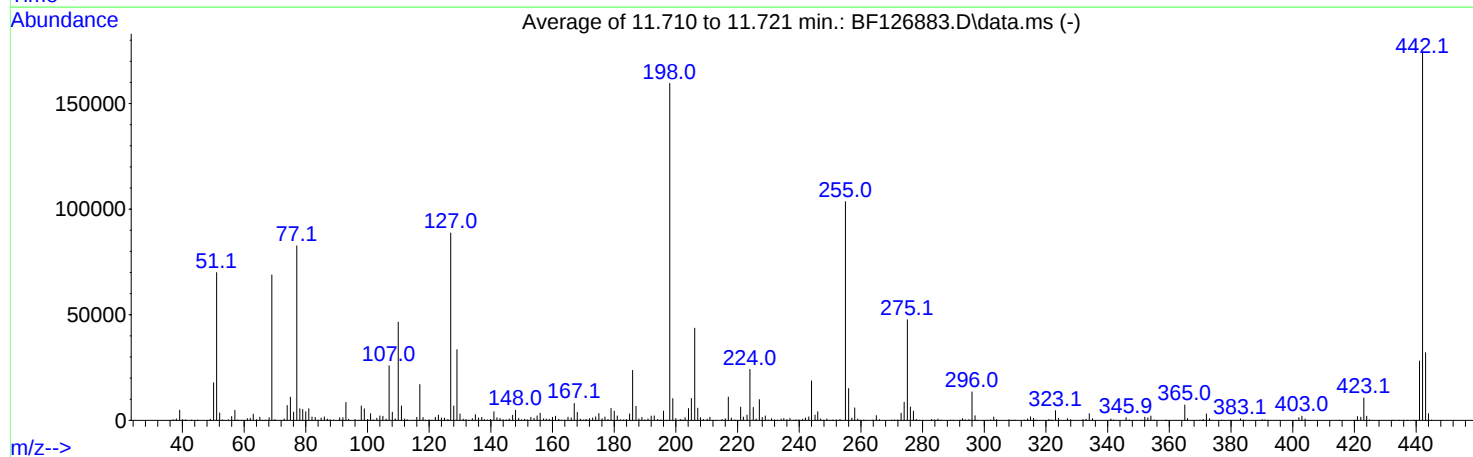


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
 Data File : BF126883.D
 Acq On : 15 Feb 2022 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 10 00:44:00 2022

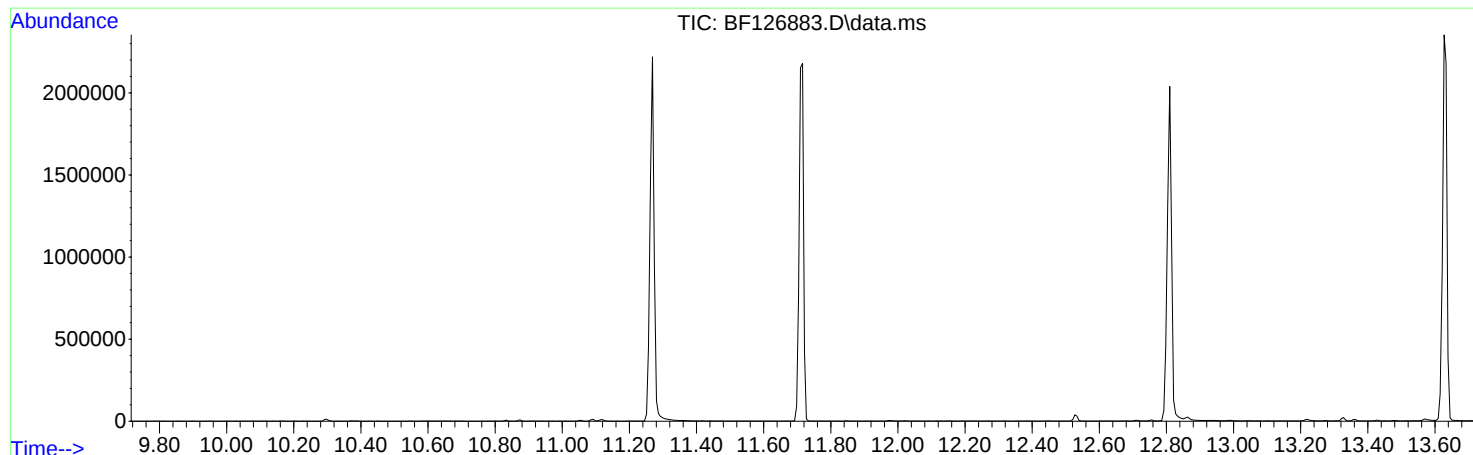




AutoFind: Scans 1602, 1603, 1604; Background Corrected with Scan 1596

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.9	70017	PASS
68	69	0.00	2	1.9	1278	PASS
69	198	0.00	100	43.2	68881	PASS
70	69	0.00	2	0.5	375	PASS
127	198	10	80	55.6	88707	PASS
197	198	0.00	2	0.1	148	PASS
198	198	100	100	100.0	159565	PASS
199	198	5	9	6.5	10292	PASS
275	198	10	60	29.9	47668	PASS
365	198	1	100	4.6	7312	PASS
441	198	0.01	100	17.6	28133	PASS
442	442	50	100	100.0	174208	PASS
443	442	15	24	18.4	32088	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\  
Data File : BF126883.D  
Acq On    : 15 Feb 2022  10:55  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 16 02:31:11 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 10 00:44:00 2022
Response via : Initial Calibration

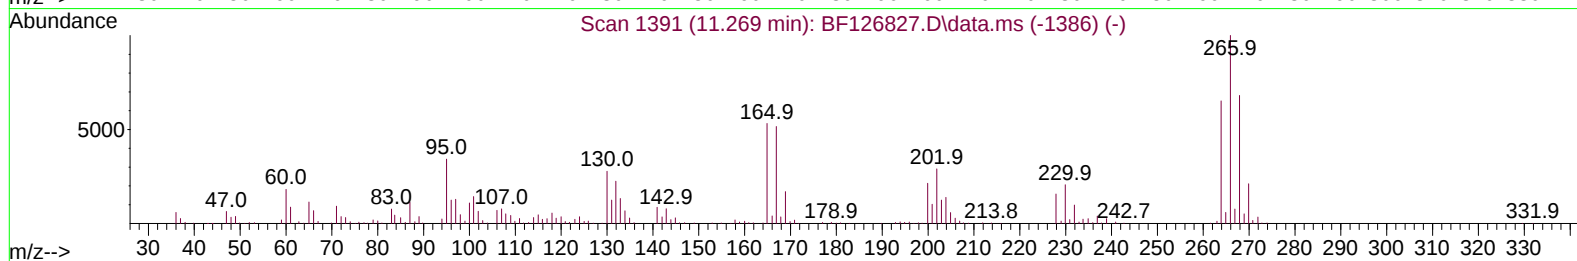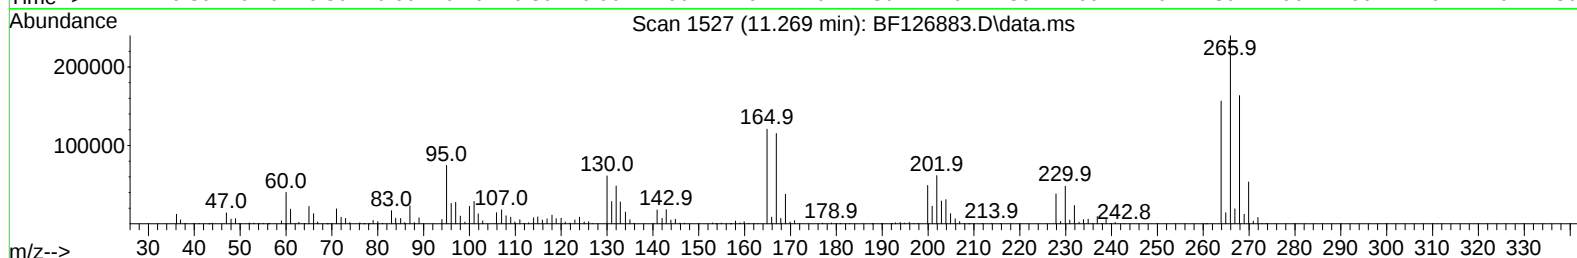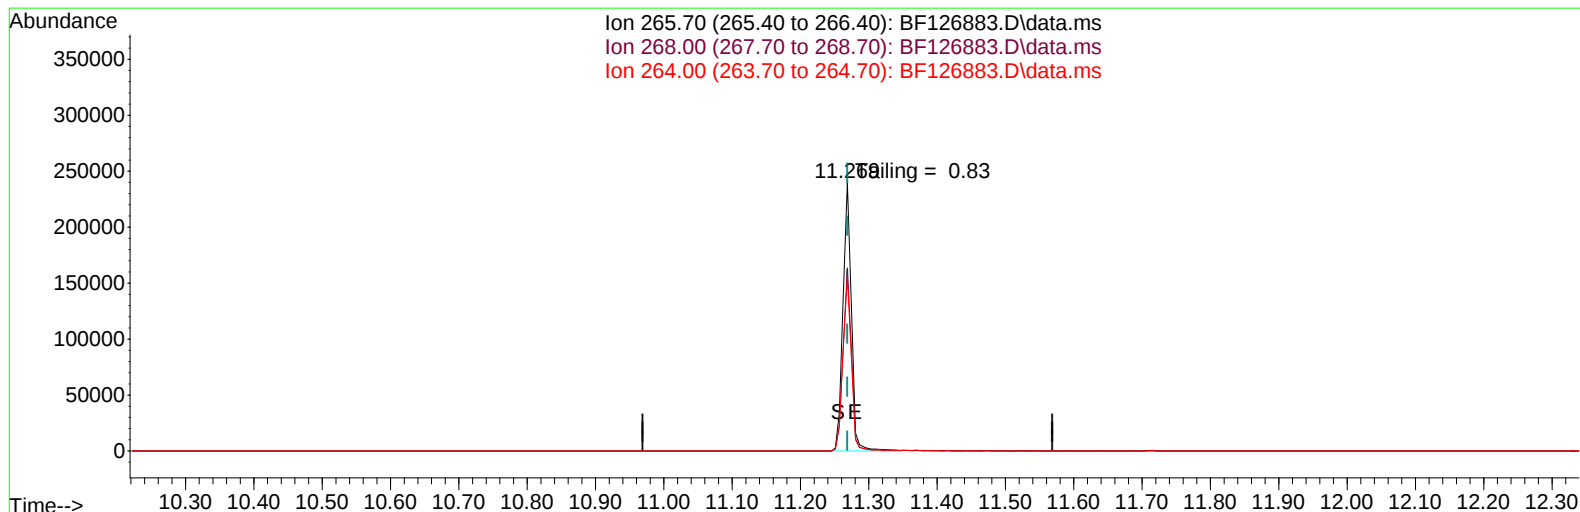

TIC: BF126883.D\data.ms

(70) Pentachlorophenol (C)

11.269min (-0.000) 251974.30 ng




response **206842**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	68.19
264.00	65.20	65.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021522\
 Data File : BF126883.D
 Acq On : 15 Feb 2022 10:55
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 02:31:11 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020922.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Feb 10 00:44:00 2022
 Response via : Initial Calibration

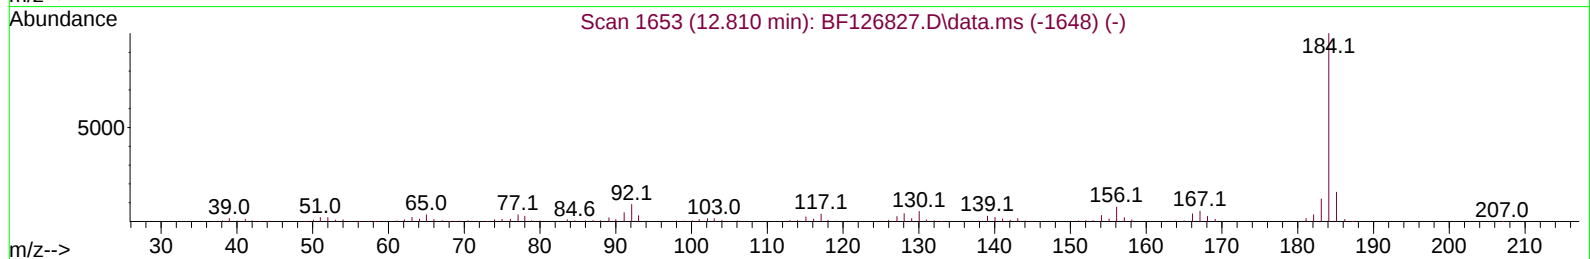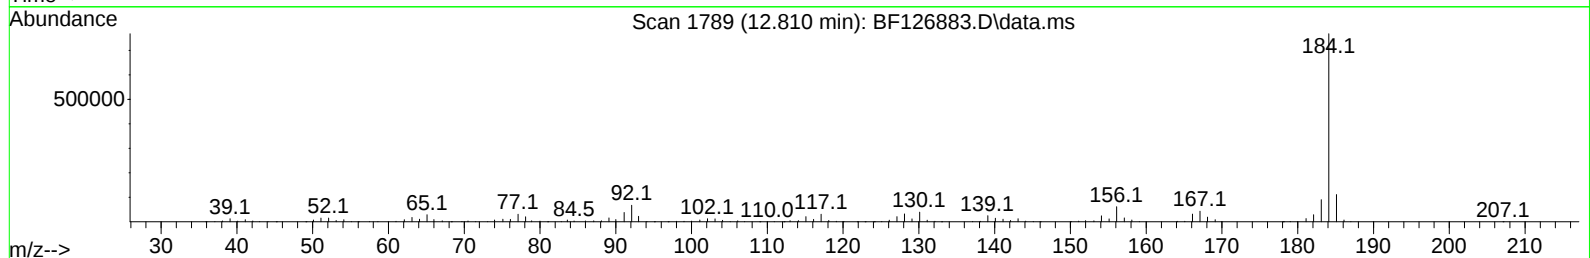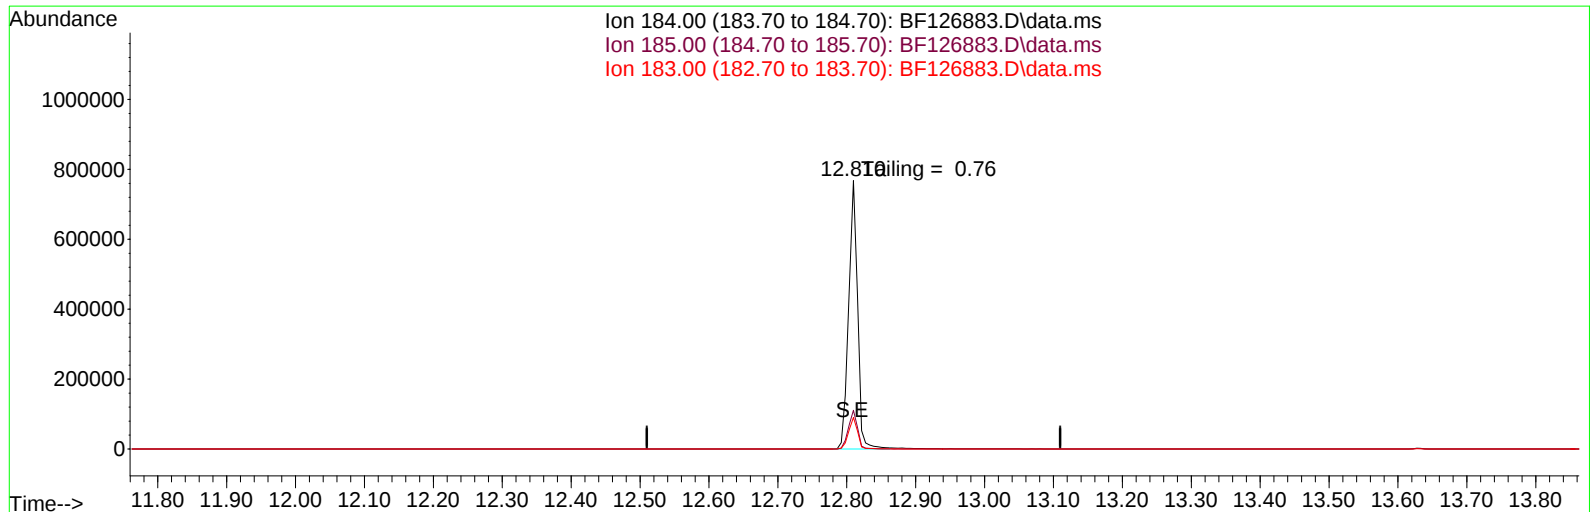

TIC: BF126883.D\data.ms

(77) Benzidine

12.810min (-12.810) 0.00 ng

response 0

Ion	Exp%	Act%
184.00	100.00	0.00
185.00	15.60	0.00#
183.00	12.00	0.00#
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/15/2022	BNA_F	<u>BF126883.D</u>
Compound Name	Response	Retention Time
DDT	371886	13.633
DDD	4926	13.327
DDE	483	12.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5409	377295	1.43

Instrument :
BNA_F
ClientSampleId :
DFTPP