
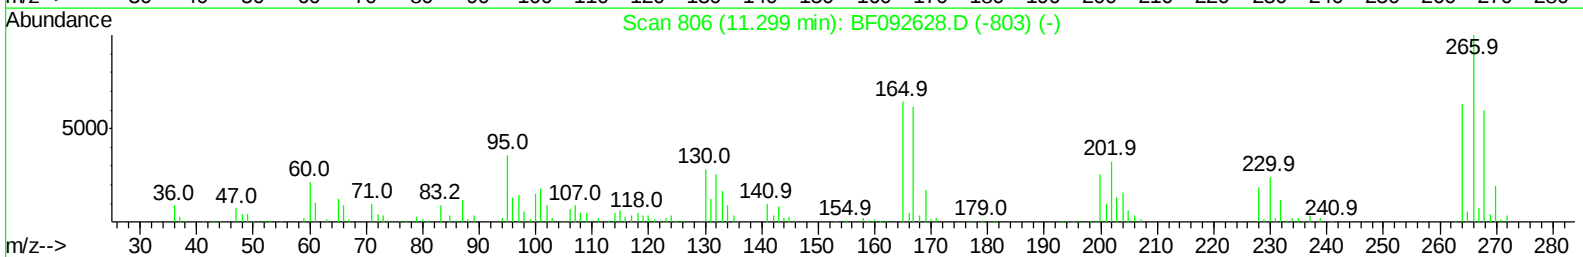
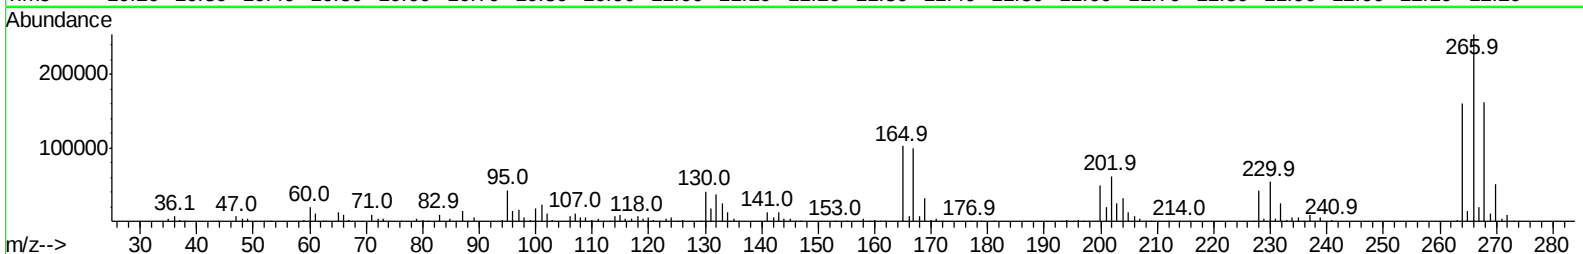


Data Path : Z:\HPCHEM1\BNA F\Data\BF021617\
Data File : BF092983.D
Acq On : 16 Feb 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 16 17:52:19 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 13 18:04:38 2017
Response via : Initial Calibration

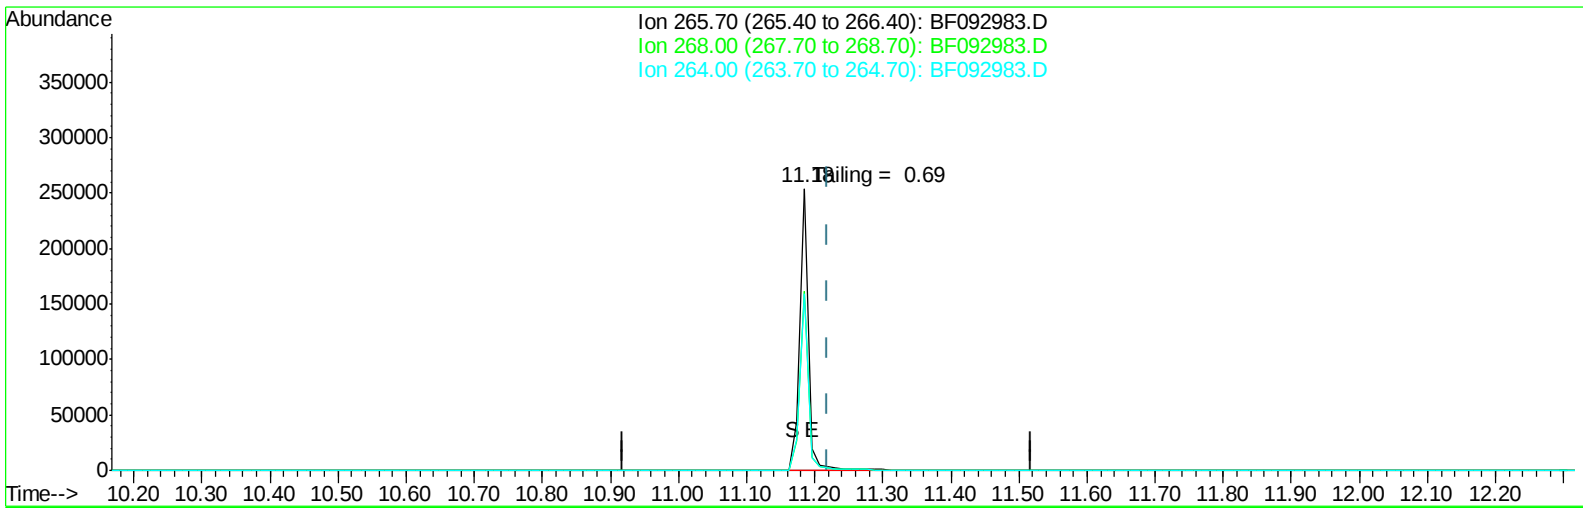

TIC: BF092983.D

(69) Pentachlorophenol (C)

11.185min (-0.034) 52743.56ng




response 229803

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.78
264.00	62.90	62.79
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF021617\
 Data File : BF092983.D
 Acq On : 16 Feb 2017 16:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 17:52:19 2017
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Feb 13 18:04:38 2017
 Response via : Initial Calibration

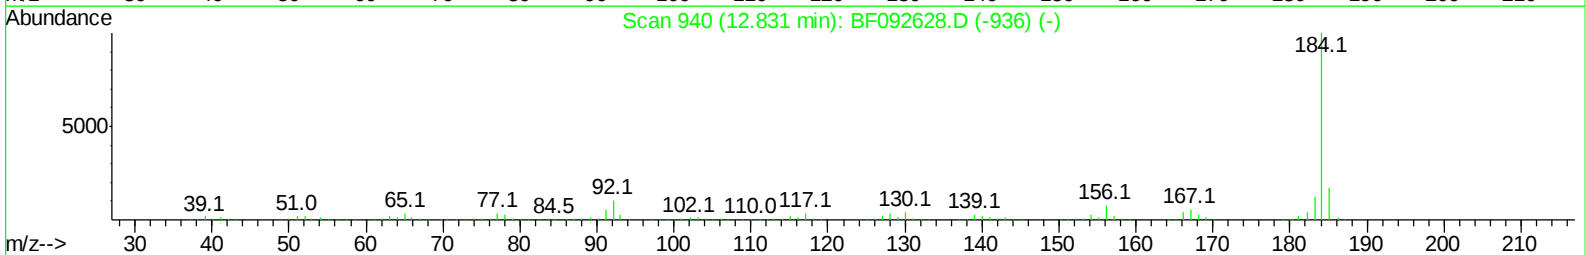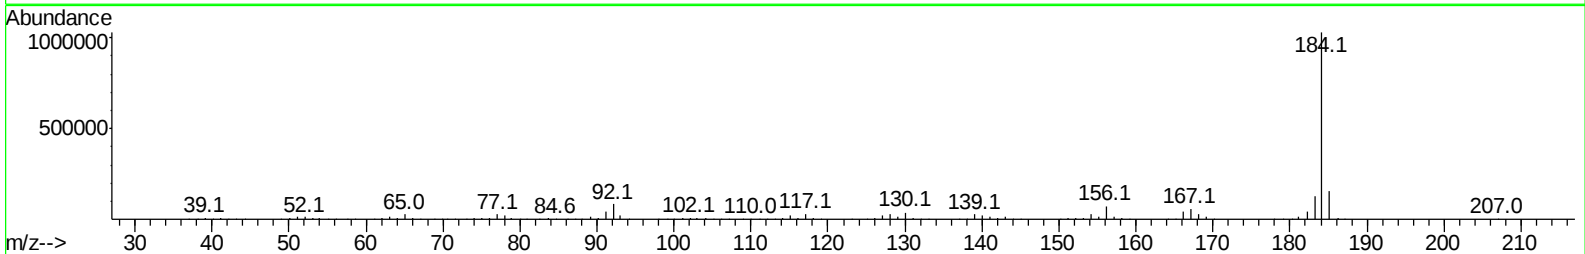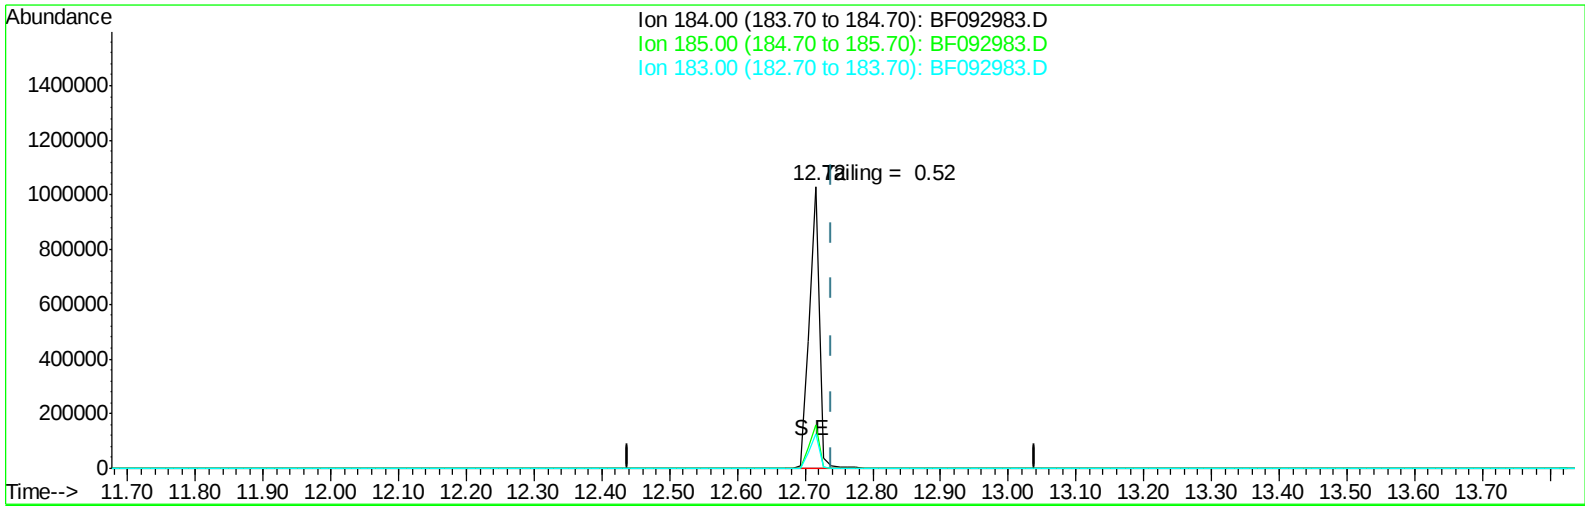

TIC: BF092983.D

(76) Benzidine

12.717min (-0.023) 0.00ng




response 1075110

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	15.35
183.00	11.50	12.48
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\Data\BF021617\
Data File : BF092983.D
Acq On : 16 Feb 2017 16:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 16 17:52:19 2017
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Feb 13 18:04:38 2017
Response via : Initial Calibration

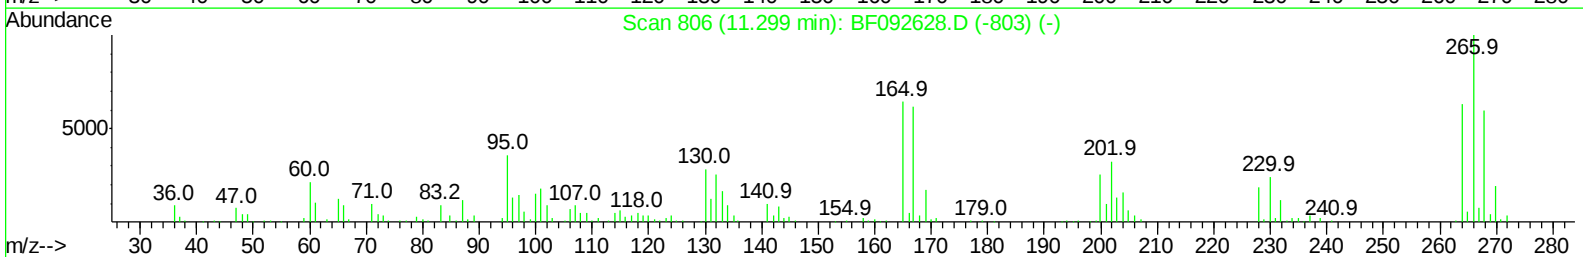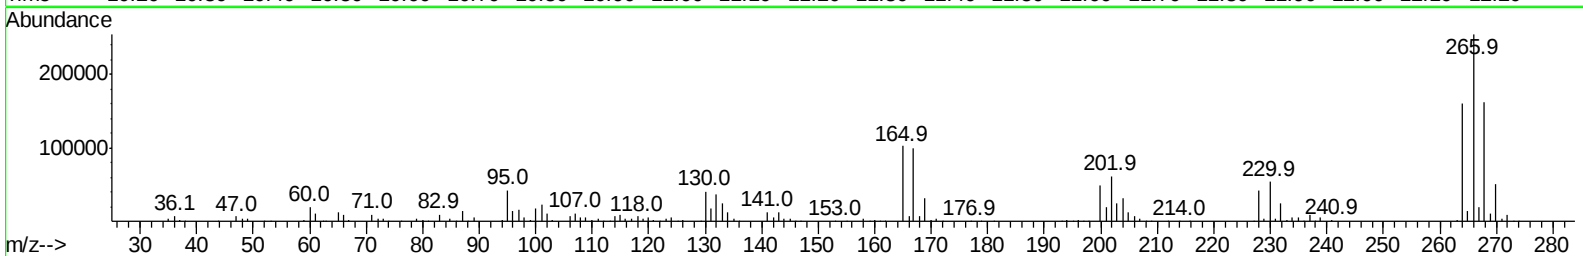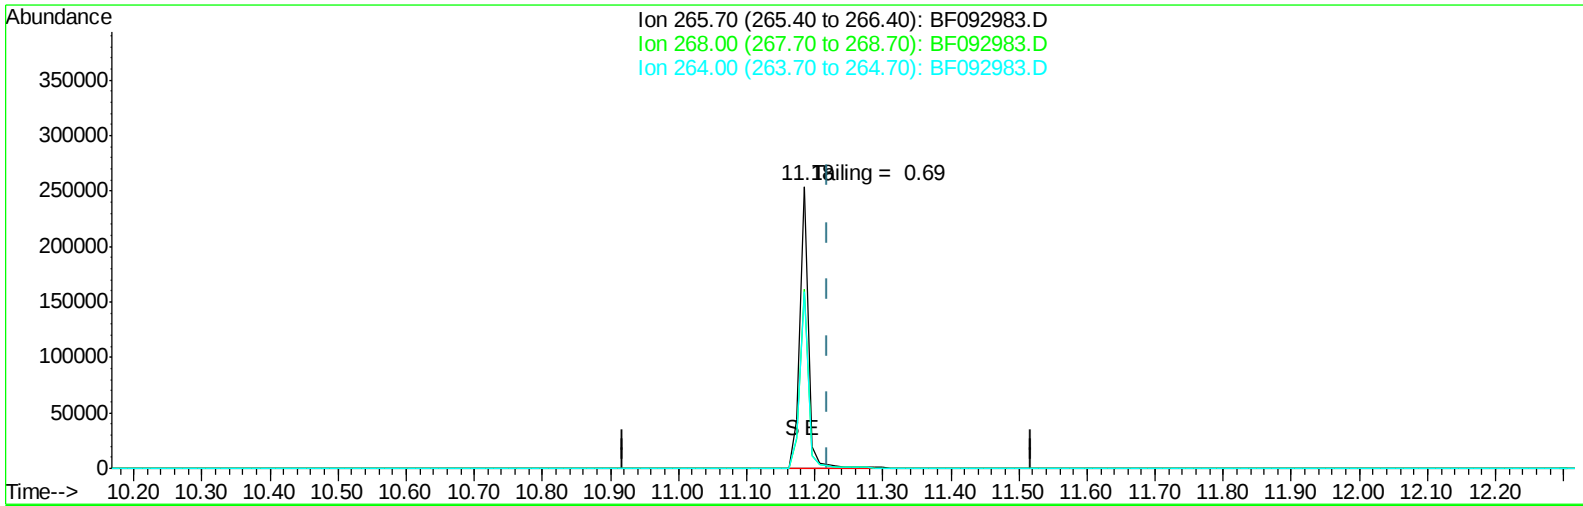

TIC: BF092983.D

(69) Pentachlorophenol (C)

11.185min (-0.034) 52743.56ng

response 229803

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	63.78
264.00	62.90	62.79
0.00	0.00	0.00