

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
 Data File : BF092985.D
 Acq On : 16 Feb 2017 17:13
 Operator : SJ/MA
 Sample : PB96992BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB96992BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.036	255	258	268	rBV	776663	1071354	26.43%	3.259%
2	5.459	292	295	298	rBV	3297260	3250737	80.20%	9.888%
3	6.499	383	386	388	rBV	3332521	3371638	83.18%	10.256%
4	6.625	395	397	400	rBV	3009145	3183988	78.55%	9.685%
5	6.853	415	417	420	rBV	599080	775507	19.13%	2.359%
6	7.013	429	431	434	rBV	2525976	2496287	61.59%	7.593%
7	7.425	464	467	469	rBV	2148843	2043206	50.41%	6.215%
8	8.145	527	530	532	rBV	1154321	1107571	27.33%	3.369%
9	9.219	621	624	626	rBV	3817120	3954037	97.55%	12.028%
10	9.893	680	683	685	rBV	1333722	1266489	31.25%	3.853%
11	10.682	749	752	754	rBV	2044736	2250809	55.53%	6.847%
12	11.368	810	812	815	rBV	1023104	1246418	30.75%	3.791%
13	12.957	948	951	954	rBV	3149143	4053258	100.00%	12.330%
14	14.008	1040	1043	1045	rBV	1535800	1407238	34.72%	4.281%
15	14.774	1107	1110	1115	rVB3	28273	55989	1.38%	0.170%
16	15.437	1165	1168	1171	rBV	1033668	1296336	31.98%	3.943%
17	16.351	1245	1248	1255	rVB4	19190	43532	1.07%	0.132%


Sum of corrected areas: 32874394

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
Data File : BF092985.D
Acq On : 16 Feb 2017 17:13
Operator : SJ/MA
Sample : PB96992BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96992BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

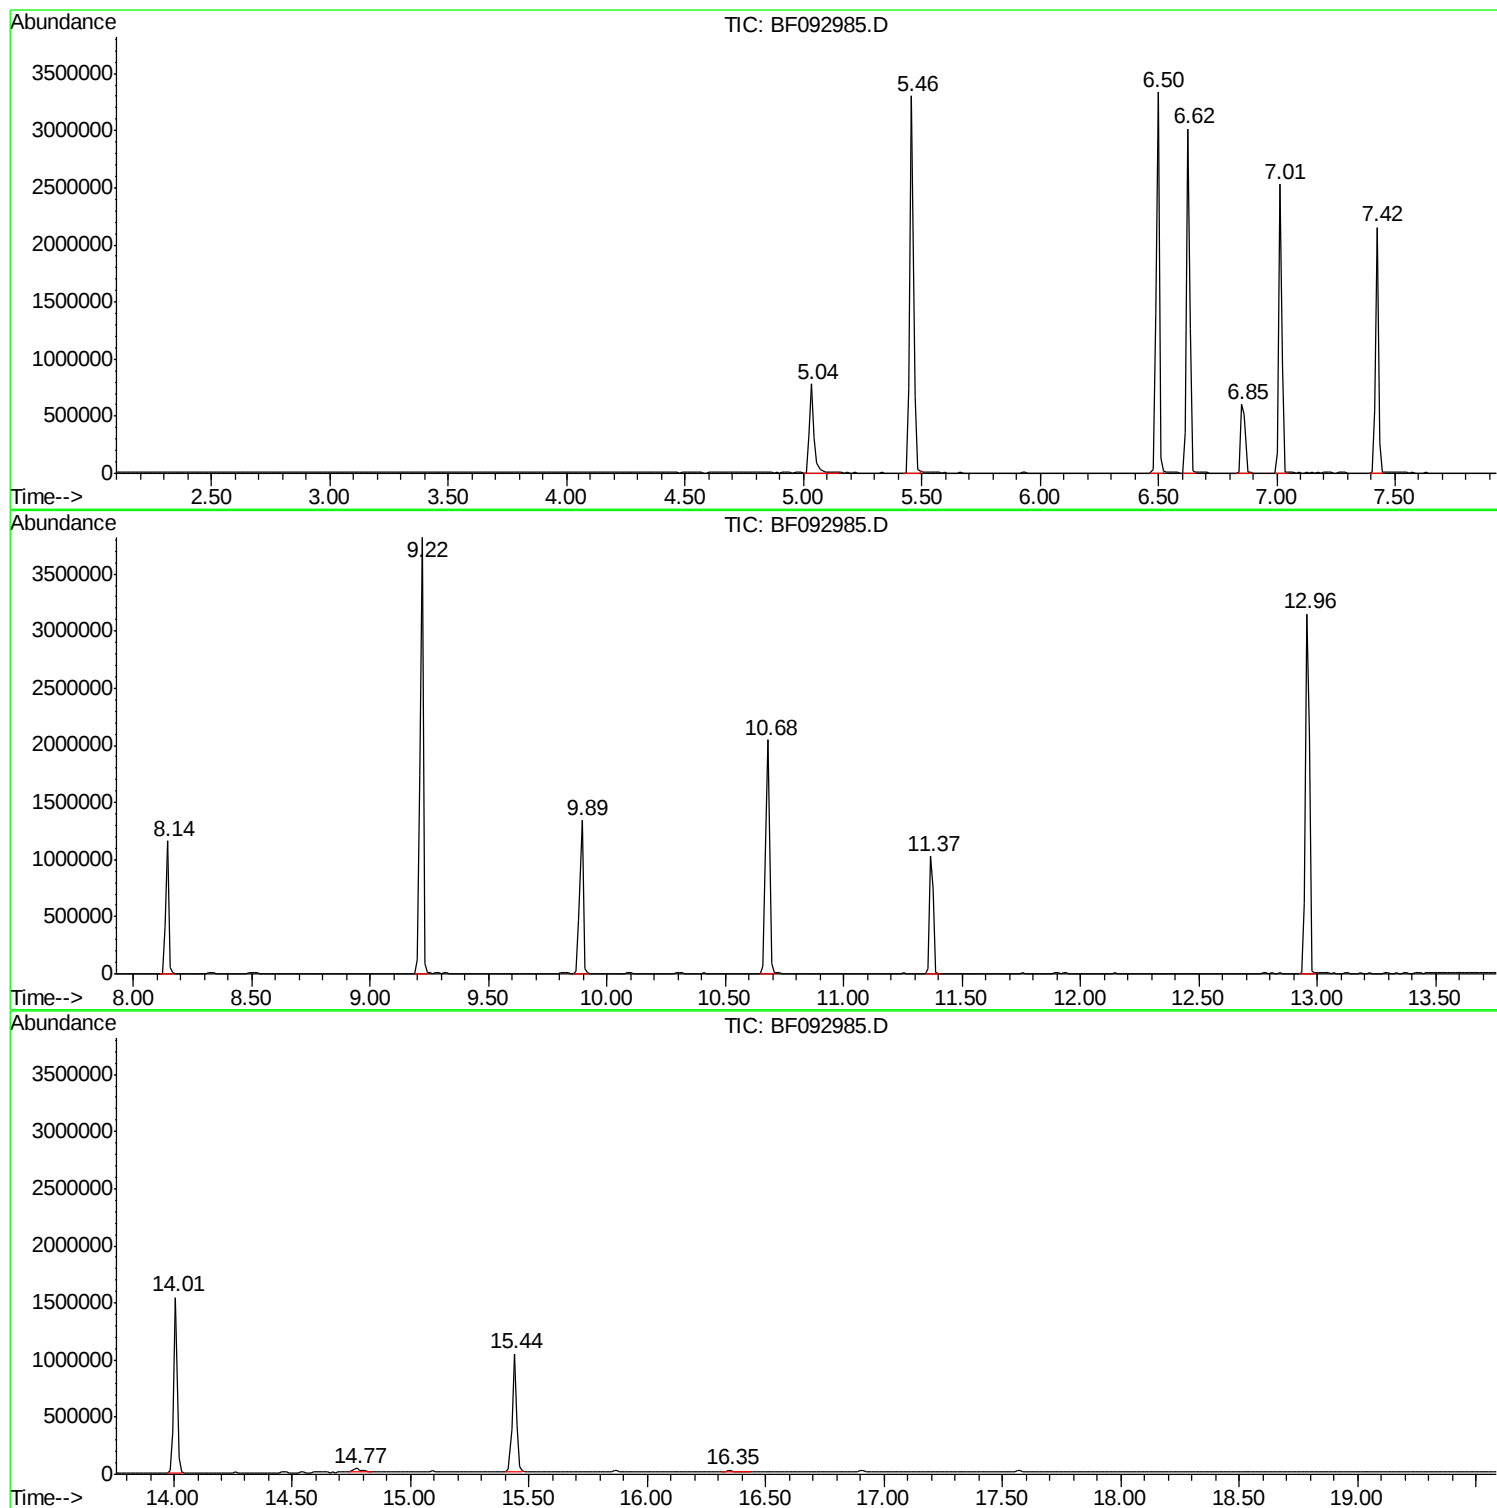

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
Data File : BF092985.D
Acq On : 16 Feb 2017 17:13
Operator : SJ/MA
Sample : PB96992BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96992BL









Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.04	27.63 ng	1071350	1,4-Dichlorobenzene-d4	6.86

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	59
2		Acetic acid, 1,1-dimethylethyl e...	116	C6H12O2	000540-88-5	39
3		Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	33
4		2-Hexanol, 2-methyl-	116	C7H16O	000625-23-0	33
5		3-Hexanol, 4-methyl-	116	C7H16O	000615-29-2	33

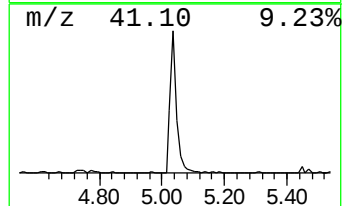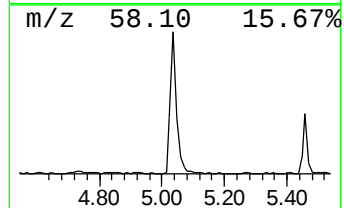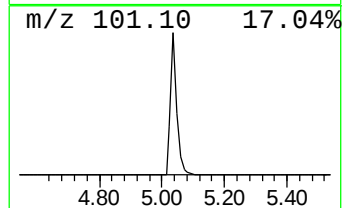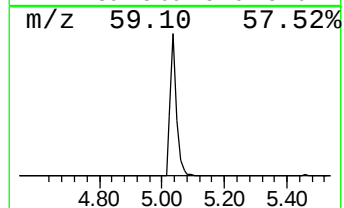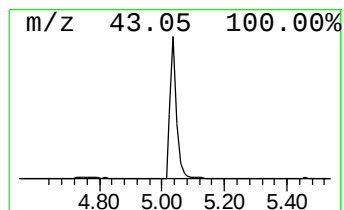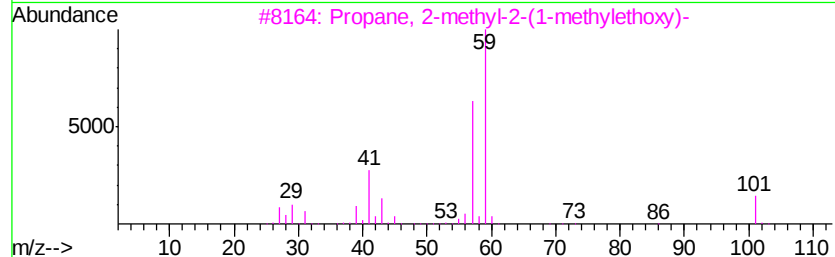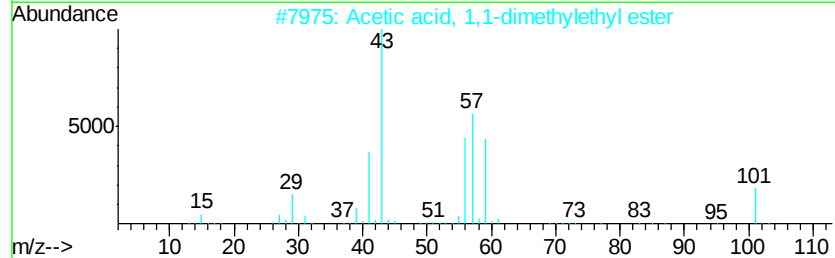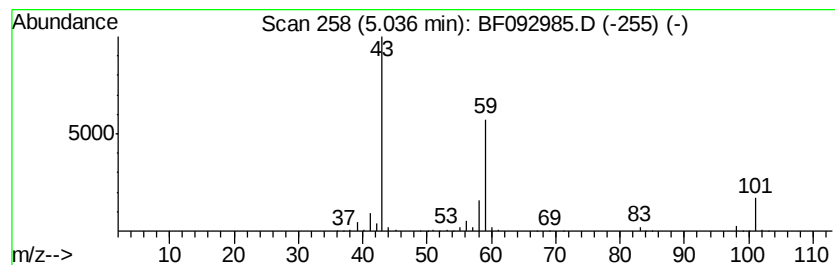

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
Data File : BF092985.D
Acq On : 16 Feb 2017 17:13
Operator : SJ/MA
Sample : PB96992BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96992BL










Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown6.62 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.62	82.11 ng	3183990	1,4-Dichlorobenzene-d4	6.86

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	3-Chloro-6-fluoro-pyrazine			132	C4H2ClFN2	1000146-10-7	27
2	5-Aminoindole			132	C8H8N2	005192-03-0	12
3	Tranylcypromine-propionyl			189	C12H15NO	1000123-86-3	10
4	Benzene, 1,3,5-trifluoro-			132	C6H3F3	000372-38-3	9
5	Bicyclo[4.2.0]octa-1,3,5-triene, ...			132	C10H12	028749-81-7	9

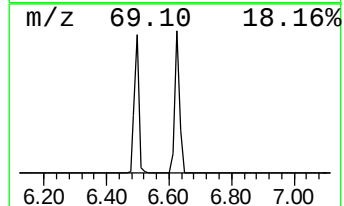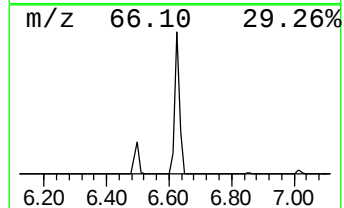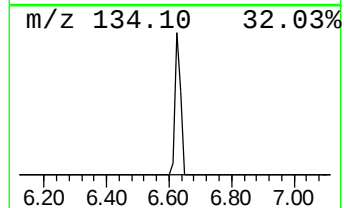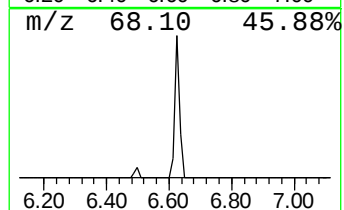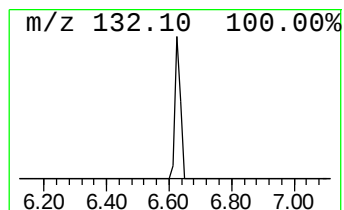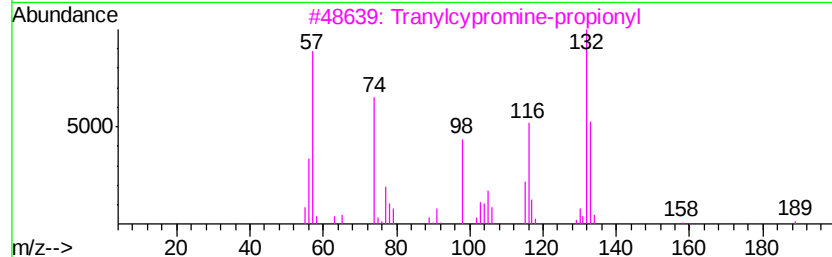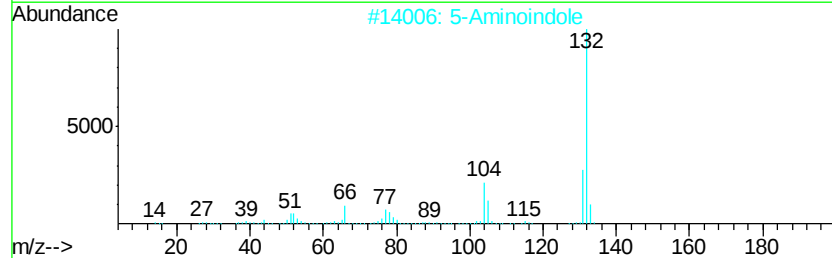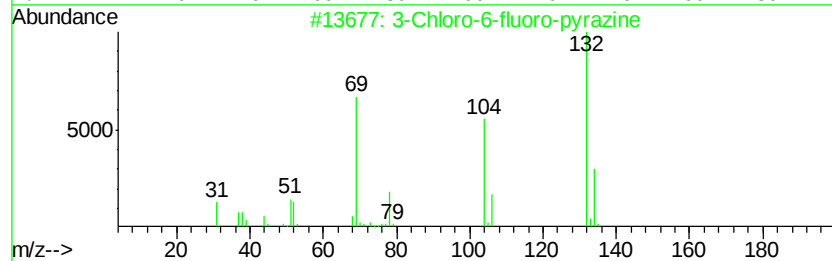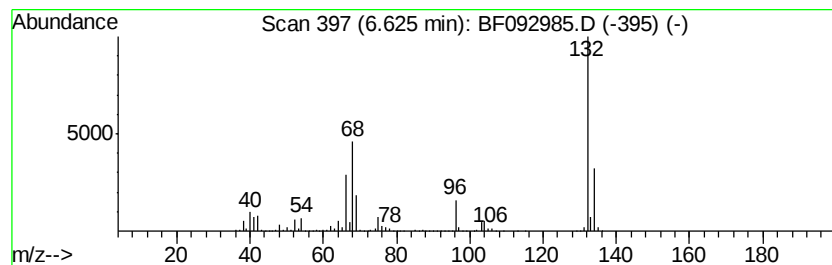

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
Data File : BF092985.D
Acq On : 16 Feb 2017 17:13
Operator : SJ/MA
Sample : PB96992BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB96992BL

Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-hy...	5.04	27.6	ng	1071350	1	6.86	775507	20.0
unknown6.62	6.62	82.1	ng	3183990	1	6.86	775507	20.0