


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021617\
 Data File : BF092983.D
 Acq On : 16 Feb 2017 16:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 13 18:04:38 2017

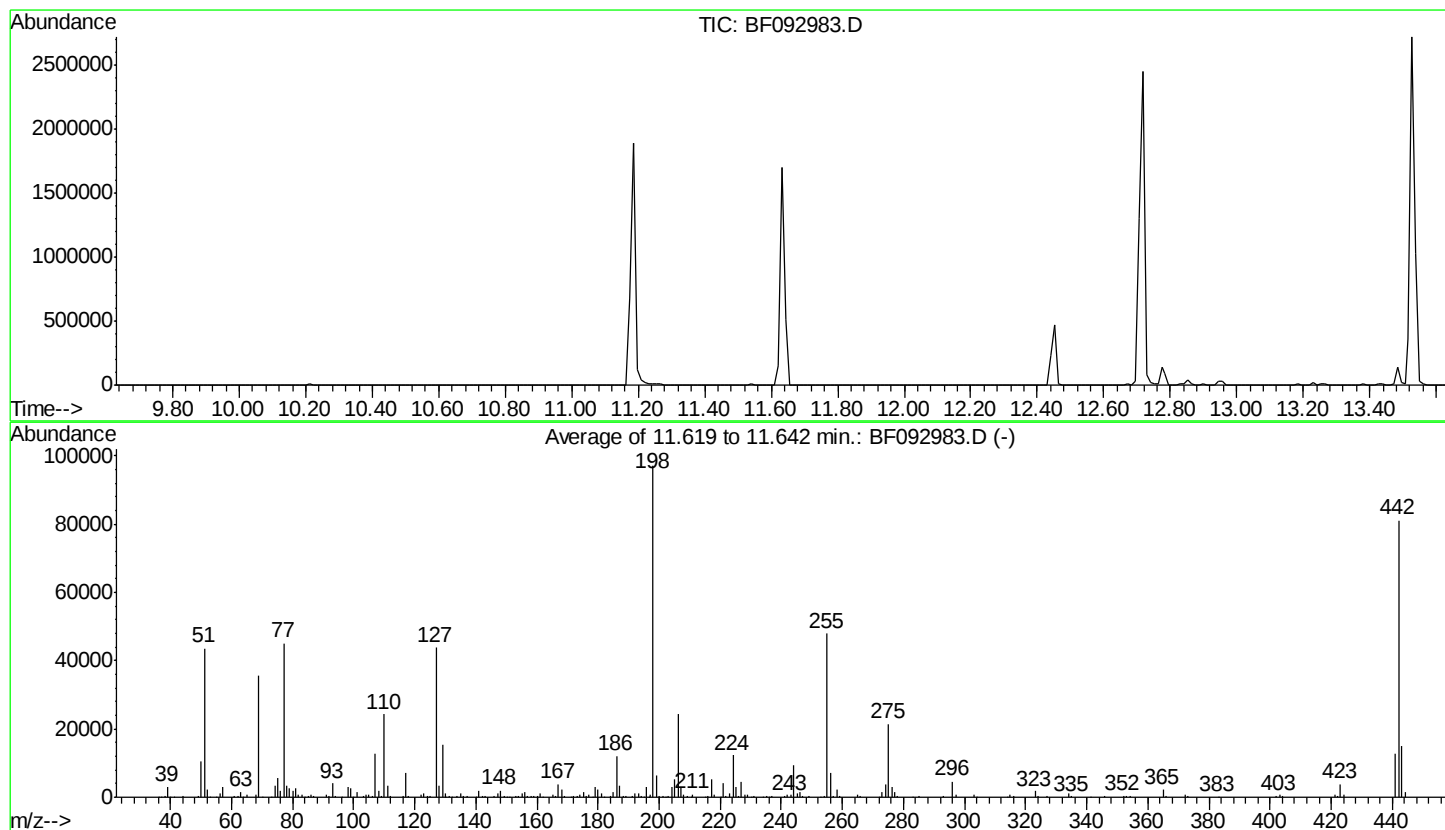

AutoFind: Scans 834, 835, 836; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.9	43630	PASS
68	69	0.00	2	1.8	630	PASS
69	198	0.00	100	36.7	35684	PASS
70	69	0.00	2	0.5	181	PASS
127	198	10	80	45.1	43851	PASS
197	198	0.00	2	0.9	867	PASS
198	198	100	100	100.0	97171	PASS
199	198	5	9	6.7	6499	PASS
275	198	10	60	22.1	21509	PASS
365	198	1	100	2.3	2196	PASS
441	442	0.01	24	15.6	12687	PASS
442	198	50	100	83.5	81186	PASS
443	442	15	24	18.5	15036	PASS