

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021622\
 Data File : BF126915.D
 Acq On : 16 Feb 2022 16:41
 Operator : CG\JU
 Sample : PB142708BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142708BL

Quant Time: Feb 17 01:07:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 14:55:48 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.928	152	122666	20.000	ng	0.00
21) Naphthalene-d8	8.210	136	513750	20.000	ng	# 0.00
39) Acenaphthene-d10	9.969	164	270152	20.000	ng	0.00
64) Phenanthrene-d10	11.463	188	503430	20.000	ng	# 0.00
76) Chrysene-d12	14.104	240	363782	20.000	ng	# 0.00
86) Perylene-d12	15.610	264	303992	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.557	112	989946	124.732	ng	0.01
7) Phenol-d6	6.551	99	1317507	123.025	ng	0.00
23) Nitrobenzene-d5	7.492	82	934861	82.135	ng	0.00
42) 2,4,6-Tribromophenol	10.763	330	391067	125.727	ng	0.00
45) 2-Fluorobiphenyl	9.292	172	1477590	80.519	ng	0.00
79) Terphenyl-d14	13.057	244	1836372	74.208	ng	0.00
Target Compounds						
						Qvalue
19) n-Nitroso-di-n-propyla...	7.492	70	127319	18.450	ng	# 81
25) Isophorone	7.492	82	933183	49.547	ng	# 69
51) 2,6-Dinitrotoluene	9.969	165	34581	8.802	ng	# 22
57) 2,4-Dinitrotoluene	9.969	165	34581	6.510	ng	# 16
67) 4-Bromophenyl-phenylether	10.763	248	23242	4.132	ng	# 1
77) Benzidine	13.057	184	26731	2.704	ng	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021622\
Data File : BF126915.D
Acq On : 16 Feb 2022 16:41
Operator : CG\JU
Sample : PB142708BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142708BL

Quant Time: Feb 17 01:07:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration




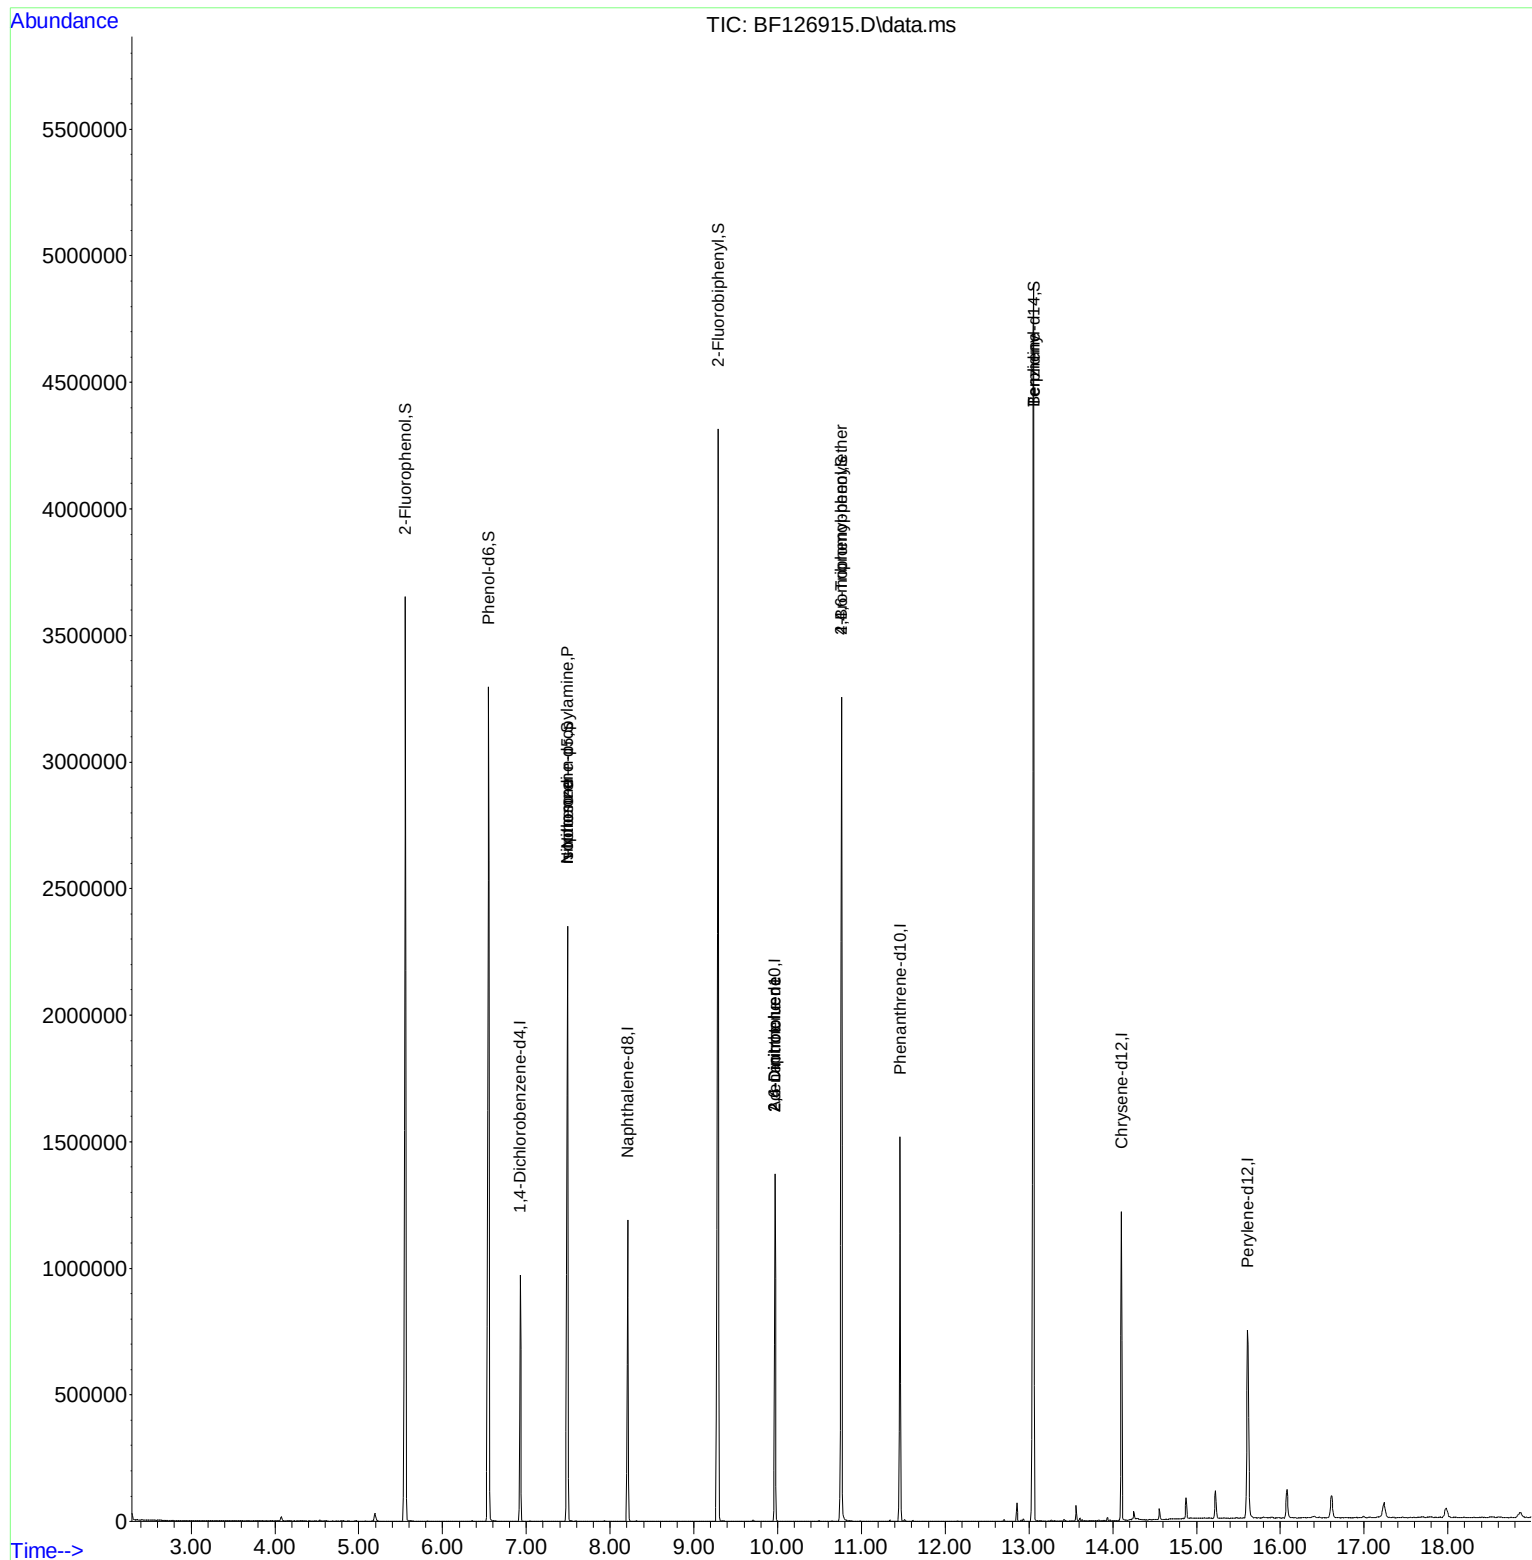


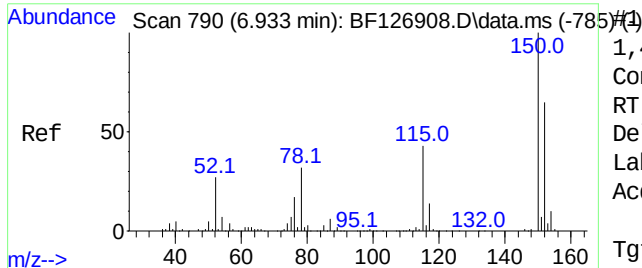

1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.928 min Scan#
Delta R.T. -0.005 min
Lab File: BF126915.D
Acq: 16 Feb 2022 16:41




Instrument :
BNA_F
ClientSampleId :
PB142708BL


Tgt Ion:152 Resp: 122666
Ion Ratio Lower Upper
152 100
150 157.3 128.1 192.1
115 70.0 56.7 85.1

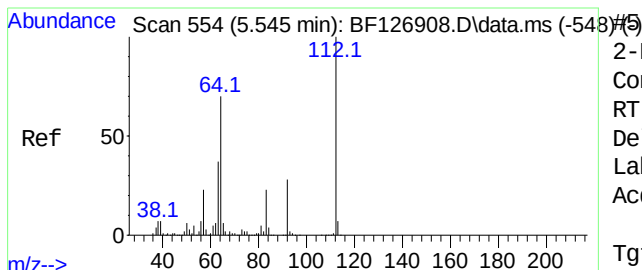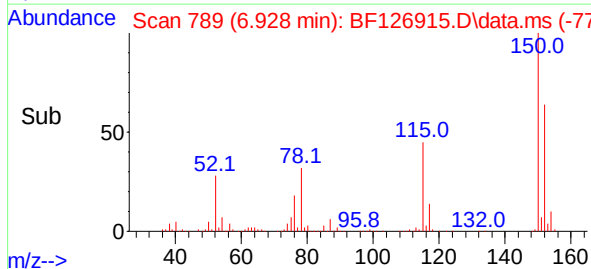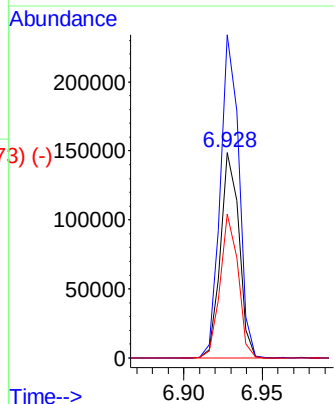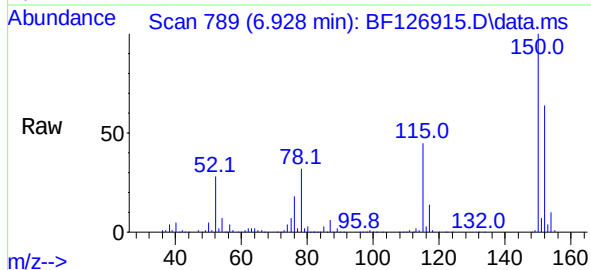

2-Fluorophenol
Concen: 124.732 ng
RT: 5.557 min Scan# 556
Delta R.T. 0.012 min
Lab File: BF126915.D
Acq: 16 Feb 2022 16:41

Tgt Ion:112 Resp: 989946
Ion Ratio Lower Upper
112 100
64 69.6 49.5 74.3
63 37.9 23.9 35.9#

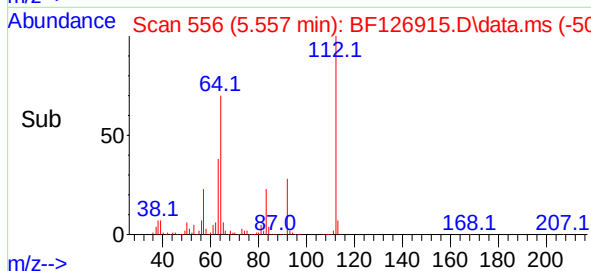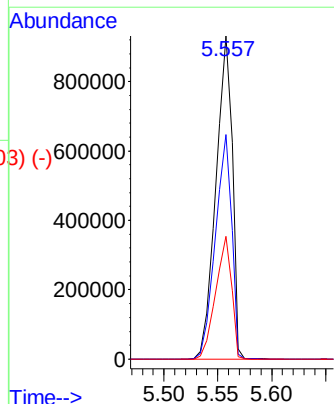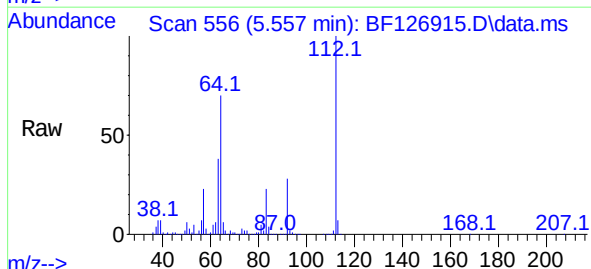

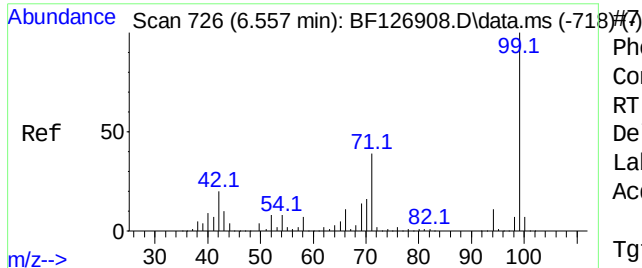

Phenol-d6

Concen: 123.025 ng

RT: 6.551 min Scan#

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL





Tgt Ion: 99 Resp: 1317507

Ion Ratio Lower Upper

99 100

42 20.1 14.2 21.4

71 39.5 24.3 36.5#

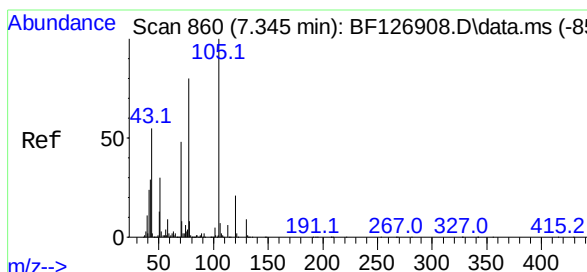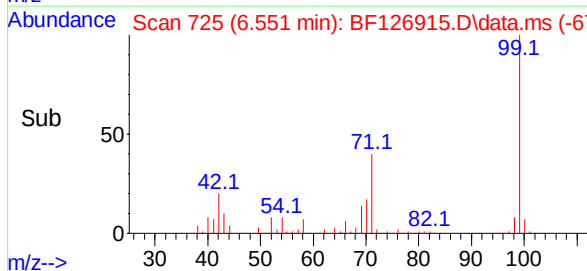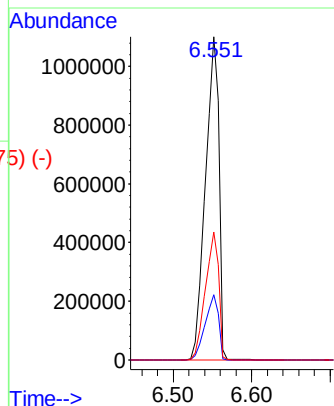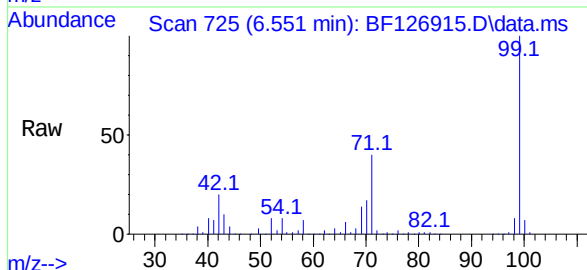

n-Nitroso-di-n-propylamine

Concen: 18.450 ng

RT: 7.492 min Scan# 885

Delta R.T. 0.147 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion: 70 Resp: 127319




Ion Ratio Lower Upper

70 100

42 47.9 45.8 68.8

101 0.0 6.9 10.3#

130 1.7 14.4 21.6#

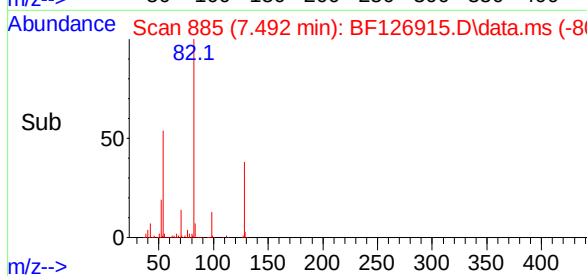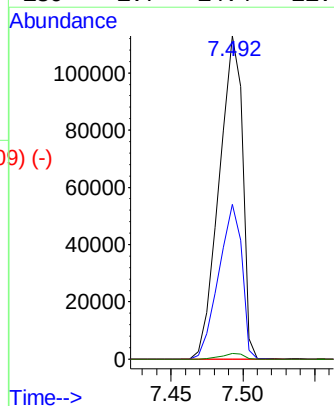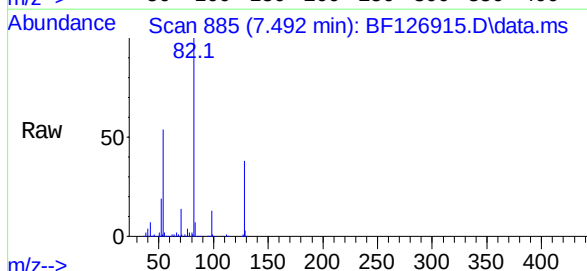

Abundance Scan 1008 (8.216 min): BF126908.D\data.ms (-10621)

Naphthalene-d8

Concen: 20.000 ng

RT: 8.210 min Scan# 1007

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL

Tgt Ion:136 Resp: 513750

Ion Ratio Lower Upper

136 100

137 11.2 8.6 13.0

54 9.6 7.8 11.6

68 6.2 6.3 9.5#

Abundance Scan 1007 (8.210 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1007 (8.210 min): BF126915.D\data.ms (-957) (-)

m/z-->

Abundance Scan 1007 (8.210 min): BF126915.D\data.ms (-957) (-)

m/z-->

Abundance

Time-->

Abundance Scan 886 (7.498 min): BF126908.D\data.ms (-880423)

Nitrobenzene-d5

Concen: 82.135 ng

RT: 7.492 min Scan# 885

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion: 82 Resp: 934861

Ion Ratio Lower Upper

82 100

128 38.5 32.7 49.1

54 54.3 41.7 62.5

Abundance Scan 885 (7.492 min): BF126915.D\data.ms

m/z-->

Abundance Scan 885 (7.492 min): BF126915.D\data.ms (-835) (-)

m/z-->

Abundance

Time-->

Abundance Scan 930 (7.757 min): BF126908.D\data.ms (-923) #25

Isophorone

Concen: 49.547 ng

RT: 7.492 min Scan# 885

Delta R.T. -0.265 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL

Tgt Ion: 82 Resp: 933183


Ion Ratio Lower Upper

82 100

95 0.0 5.0 7.4#


138 0.0 12.3 18.5#

Abundance Scan 885 (7.492 min): BF126915.D\data.ms

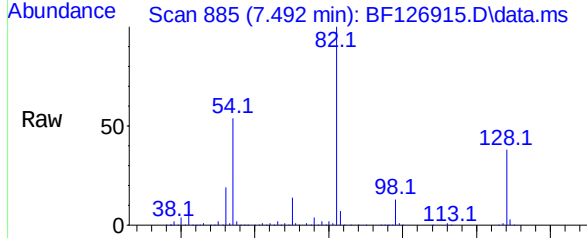


m/z-->

Abundance Scan 885 (7.492 min): BF126915.D\data.ms (-879) (-)

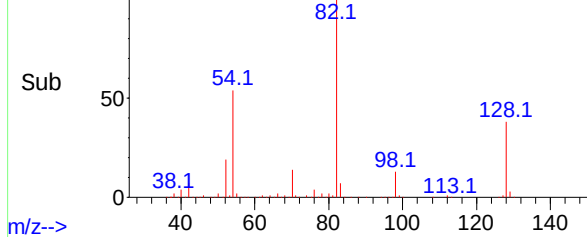

m/z-->

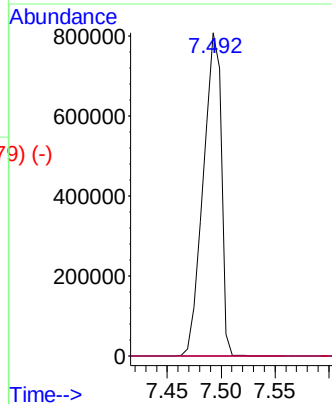

Abundance Scan 1307 (9.974 min): BF126908.D\data.ms (-1306) #39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.969 min Scan# 1306

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion:164 Resp: 270152


Ion Ratio Lower Upper

164 100

162 98.1 81.4 122.0


160 44.0 36.6 54.8

Abundance Scan 1306 (9.969 min): BF126915.D\data.ms

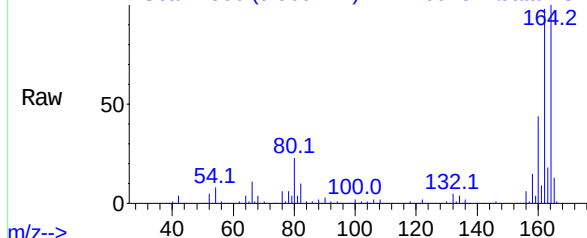


m/z-->

Abundance Scan 1306 (9.969 min): BF126915.D\data.ms (-1256) (-)

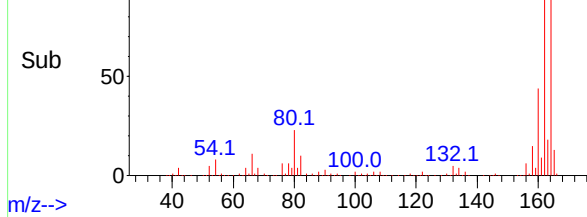

m/z-->

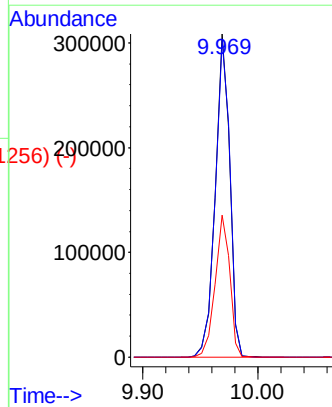

Abundance Scan 1442 (10.769 min): BF126908.D\data.ms (-1463) (-)

2,4,6-Tribromophenol

Concen: 125.727 ng

RT: 10.763 min Scan# 1442

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL

Tgt Ion:330 Resp: 391067

Ion Ratio Lower Upper

330 100

332 95.5 76.0 114.0

141 35.5 30.1 45.1

Abundance Scan 1441 (10.763 min): BF126915.D\data.ms

m/z-->

Ref

62.0 102.9 140.9 221.9 329.8

Raw

62.0 102.9 141.0 182.8 221.9 329.8

m/z-->

Abundance Scan 1441 (10.763 min): BF126915.D\data.ms (-1391) (-)

m/z-->

Sub

62.0 102.9 141.0 182.8 221.9 329.8

m/z-->

Abundance

10.763

400000

300000

200000

100000

0

Time-->

Abundance Scan 1191 (9.292 min): BF126908.D\data.ms (-1184) (-)

2-Fluorobiphenyl

Concen: 80.519 ng

RT: 9.292 min Scan# 1191

Delta R.T. 0.000 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion:172 Resp: 1477590

Ion Ratio Lower Upper

172 100

171 34.7 28.3 42.5

170 23.2 19.0 28.6

Abundance Scan 1191 (9.292 min): BF126915.D\data.ms

m/z-->

Ref

51.0 85.1 120.1 146.1 172.1

Raw

39.1 63.1 85.1 105.0 125.1 146.1 172.1

m/z-->

Abundance Scan 1191 (9.292 min): BF126915.D\data.ms (-1140) (-)

m/z-->

Sub

39.1 63.1 85.1 105.0 125.1 146.1 172.1

m/z-->

Abundance

9.292


1000000

500000

0

Time-->

Abundance Scan 1270 (9.757 min): BF126908.D\data.ms (-1264)

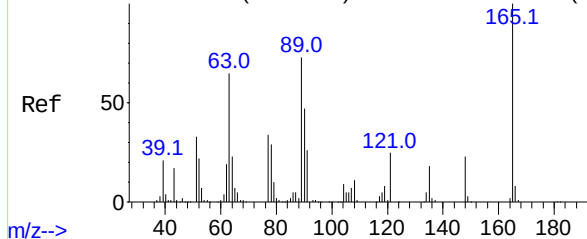

2,6-Dinitrotoluene

Concen: 8.802 ng

RT: 9.969 min Scan# 1306

Delta R.T. 0.212 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL



Tgt Ion:165 Resp: 34581

Ion Ratio Lower Upper


165 100

63 1.8 48.4 72.6#


89 1.5 50.5 75.7#

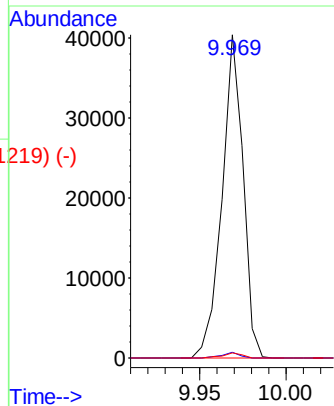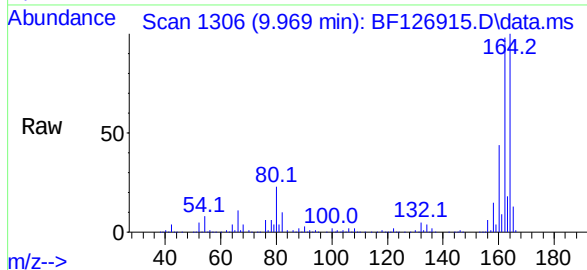

Abundance Scan 1306 (9.969 min): BF126915.D\data.ms (-1219) (-)

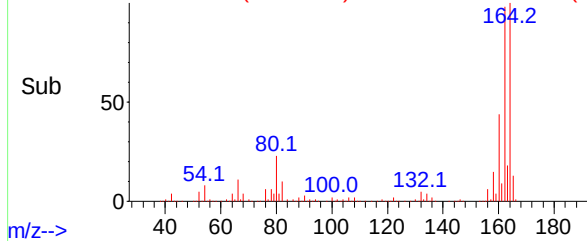

Abundance Scan 1339 (10.163 min): BF126908.D\data.ms (-1357) (-)

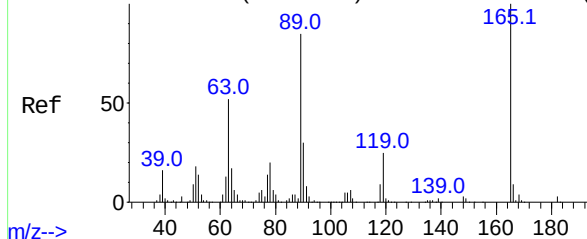

2,4-Dinitrotoluene

Concen: 6.510 ng

RT: 9.969 min Scan# 1306

Delta R.T. -0.194 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion:165 Resp: 34581



Ion Ratio Lower Upper

165 100


63 1.8 43.0 64.6#

89 1.5 71.0 106.4#


182 0.0 1.6 2.4#

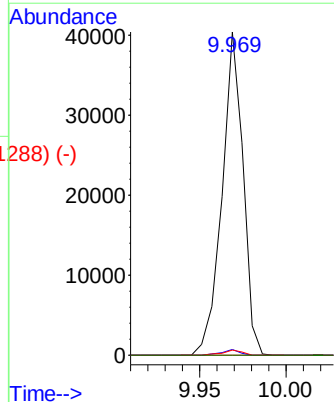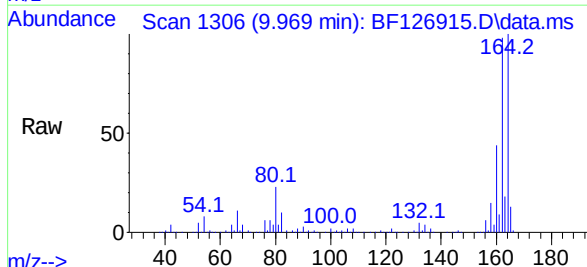

Abundance Scan 1306 (9.969 min): BF126915.D\data.ms (-1288) (-)

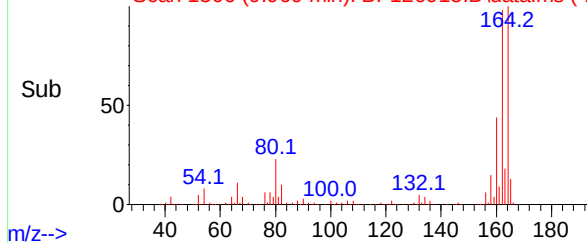




Abundance Scan 1560 (11.463 min): BF126908.D\data.ms (-1560) (-)

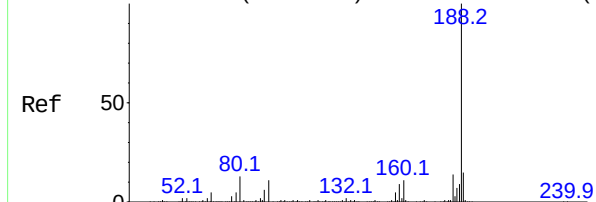


Phenanthrene-d10
Concen: 20.000 ng
RT: 11.463 min Scan# 1560
Delta R.T. 0.000 min
Lab File: BF126915.D
Acq: 16 Feb 2022 16:41

Instrument :
BNA_F
ClientSampleId :
PB142708BL

Tgt Ion:188 Resp: 503430
Ion Ratio Lower Upper
188 100
94 10.0 10.1 15.1#
80 11.6 11.8 17.6#

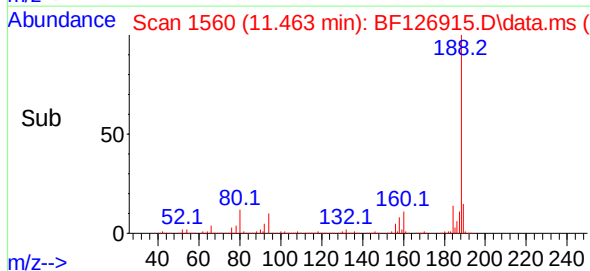
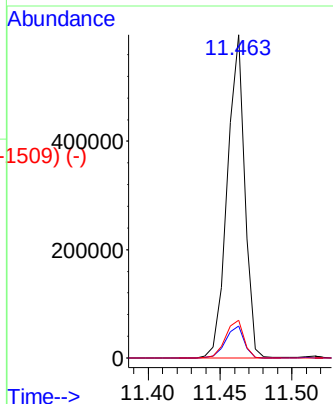
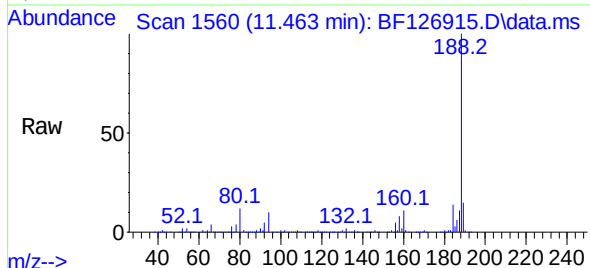


Abundance Scan 1482 (11.004 min): BF126908.D\data.ms (-1482) (-)

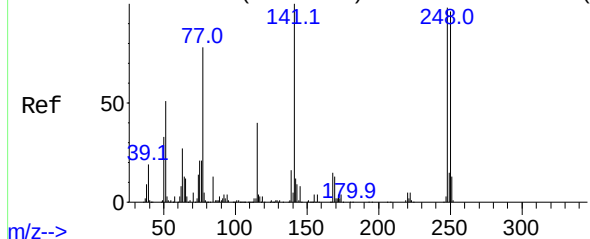

4-Bromophenyl-phenylether
Concen: 4.132 ng
RT: 10.763 min Scan# 1441
Delta R.T. -0.241 min
Lab File: BF126915.D
Acq: 16 Feb 2022 16:41

Tgt Ion:248 Resp: 23242
Ion Ratio Lower Upper
248 100
250 185.0 76.2 114.4#
141 537.4 66.2 99.4#

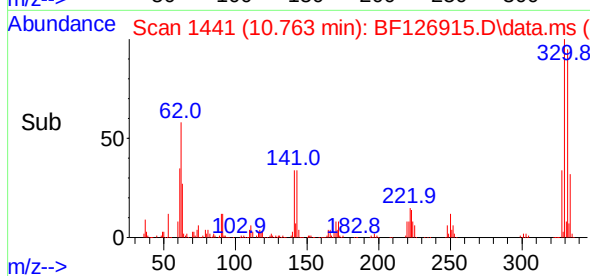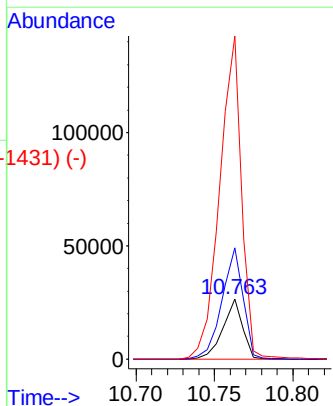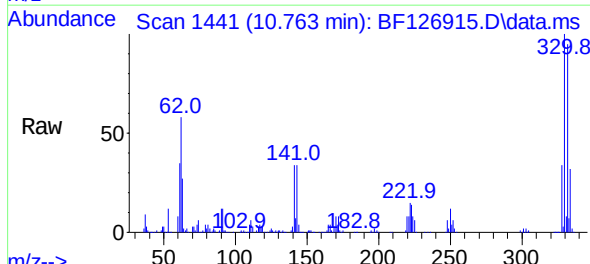

Abundance Scan 2010 (14.110 min): BF126908.D\data.ms (-2074) (-)

Chrysene-d12

Concen: 20.000 ng

RT: 14.104 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL

Tgt Ion:240 Resp: 363782

Ion Ratio Lower Upper

240 100

120 12.9 14.4 21.6#

236 26.0 20.5 30.7

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance Scan 2009 (14.104 min): BF126915.D\data.ms (-1959) (-)

m/z-->

Abundance

400000

300000

200000

100000

0

14.104

14.10

14.20

Time-->

Abundance Scan 1787 (12.798 min): BF126908.D\data.ms (-1787) (-)

Benzidine

Concen: 2.704 ng

RT: 13.057 min Scan# 1831

Delta R.T. 0.259 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion:184 Resp: 26731

Ion Ratio Lower Upper

184 100

185 15.4 11.8 17.8

183 10.2 8.2 12.2

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance

20000

10000

0

13.057

13.00

13.05

Time-->

Abundance Scan 1830 (13.051 min): BF126908.D\data.ms (-1879) (-)

Terphenyl-d14

Concen: 74.208 ng

RT: 13.057 min Scan# 1830

Delta R.T. 0.006 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Instrument :

BNA_F

ClientSampleId :

PB142708BL

Tgt Ion:244 Resp: 1836372

Ion Ratio Lower Upper

244 100

212 6.8 5.0 7.4

122 9.9 13.3 19.9#

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance Scan 1831 (13.057 min): BF126915.D\data.ms

m/z-->

Abundance

13.057

1500000

1000000

500000

0

Time-->

13.00 13.10 13.20

Abundance Scan 2265 (15.609 min): BF126908.D\data.ms (-2286) (-)

Perylene-d12

Concen: 20.000 ng

RT: 15.610 min Scan# 2265

Delta R.T. 0.000 min

Lab File: BF126915.D

Acq: 16 Feb 2022 16:41

Tgt Ion:264 Resp: 303992

Ion Ratio Lower Upper

264 100

260 23.6 19.2 28.8

265 21.0 17.4 26.2

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance Scan 2265 (15.610 min): BF126915.D\data.ms

m/z-->

Abundance

15.610

200000

150000

100000

50000

0

Time-->

15.60 15.70