
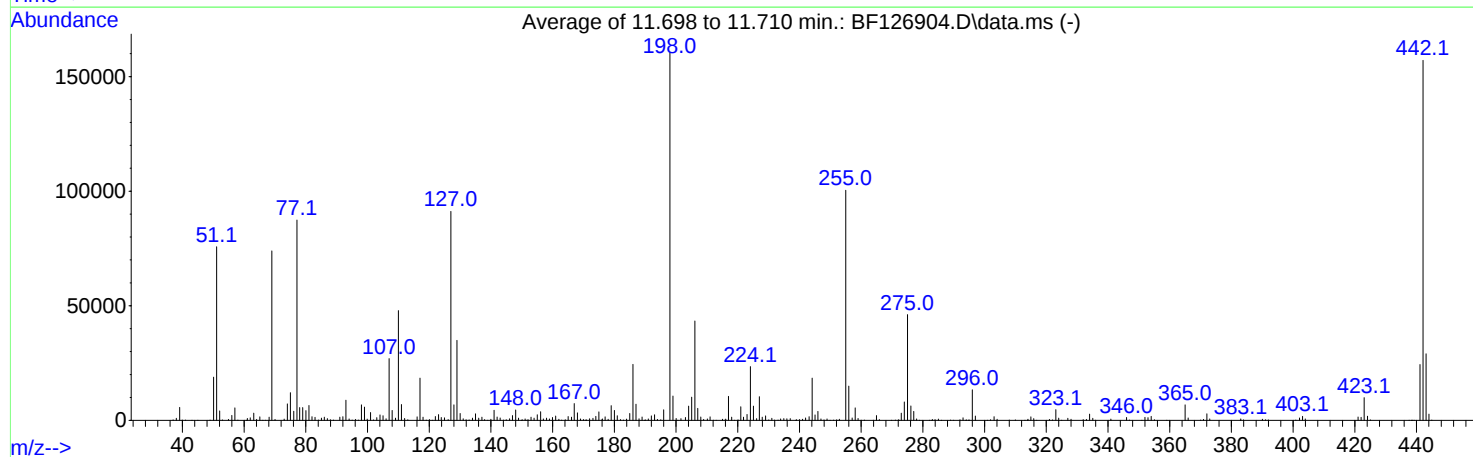


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021622\
 Data File : BF126904.D
 Acq On : 16 Feb 2022 10:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 16 14:55:48 2022

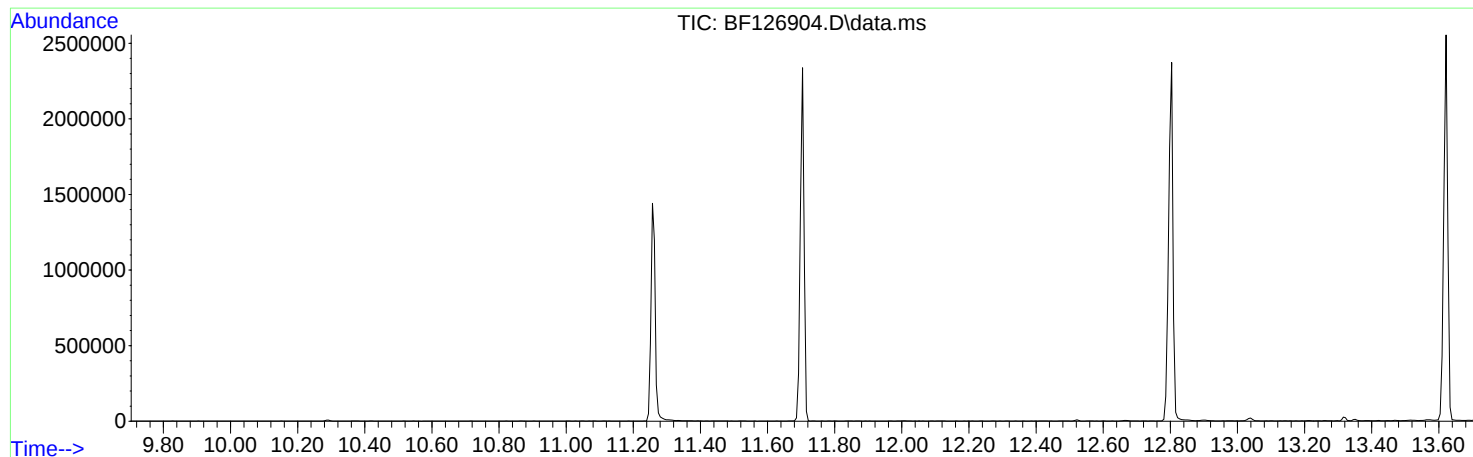


AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.2	75749	PASS
68	69	0.00	2	1.9	1422	PASS
69	198	0.00	100	46.1	73960	PASS
70	69	0.00	2	0.5	401	PASS
127	198	10	80	56.8	91197	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	160517	PASS
199	198	5	9	6.6	10618	PASS
275	198	10	60	28.7	46139	PASS
365	198	1	100	4.2	6772	PASS
441	198	0.01	100	15.2	24365	PASS
442	442	50	100	100.0	157091	PASS
443	442	15	24	18.5	29032	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021622\
Data File : BF126904.D
Acq On : 16 Feb 2022 10:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 16 12:19:25 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 12:11:22 2022
Response via : Initial Calibration

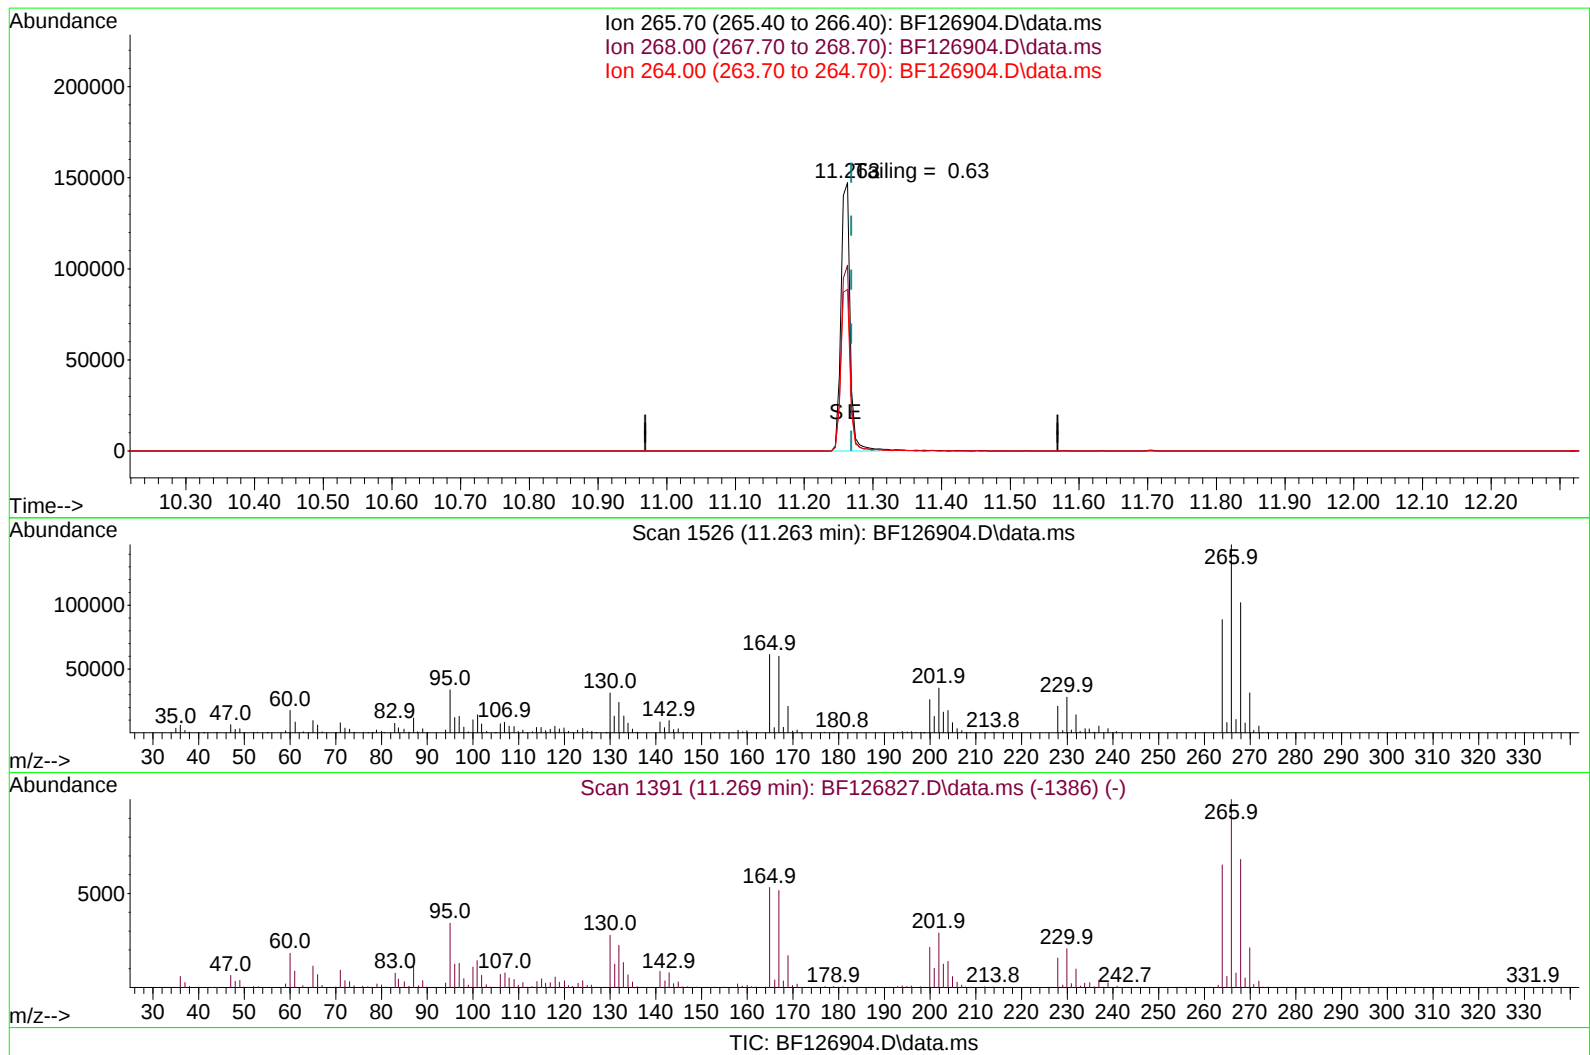

(70) Pentachlorophenol (C)

11.263min (-0.006) 25914.00 ng




response 135842

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	68.10	69.21
264.00	65.20	60.22
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021622\
 Data File : BF126904.D
 Acq On : 16 Feb 2022 10:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 16 12:19:25 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 12:11:22 2022
 Response via : Initial Calibration

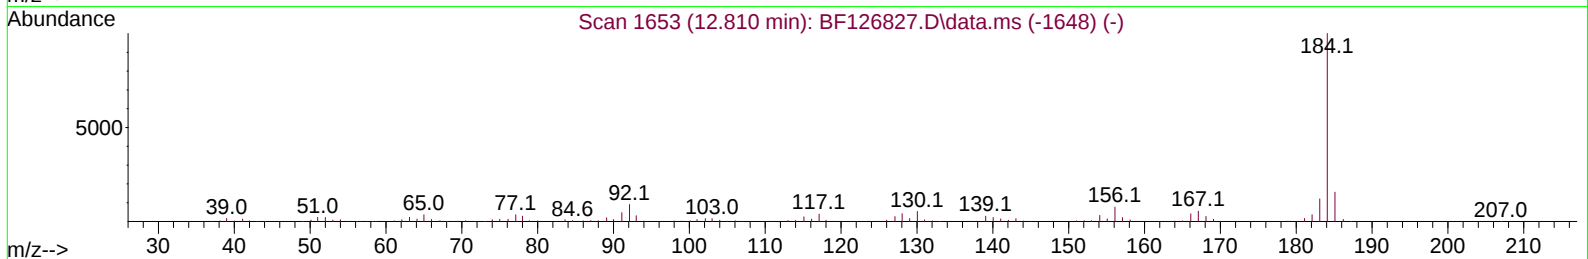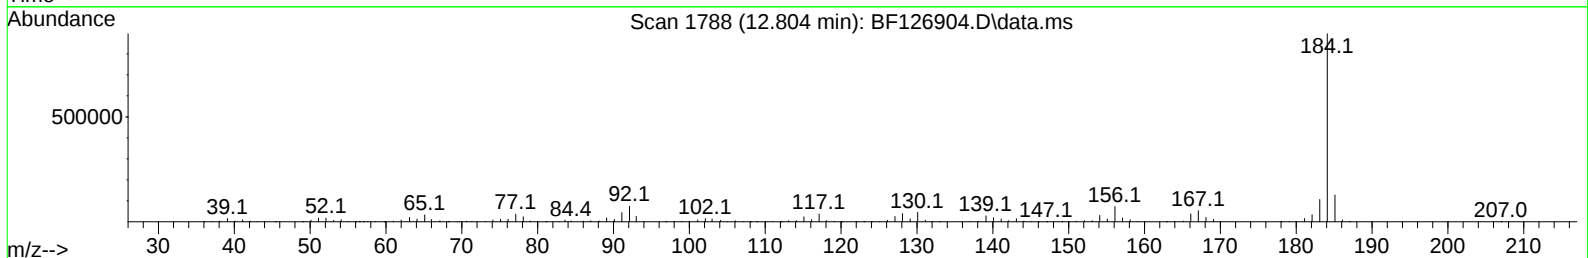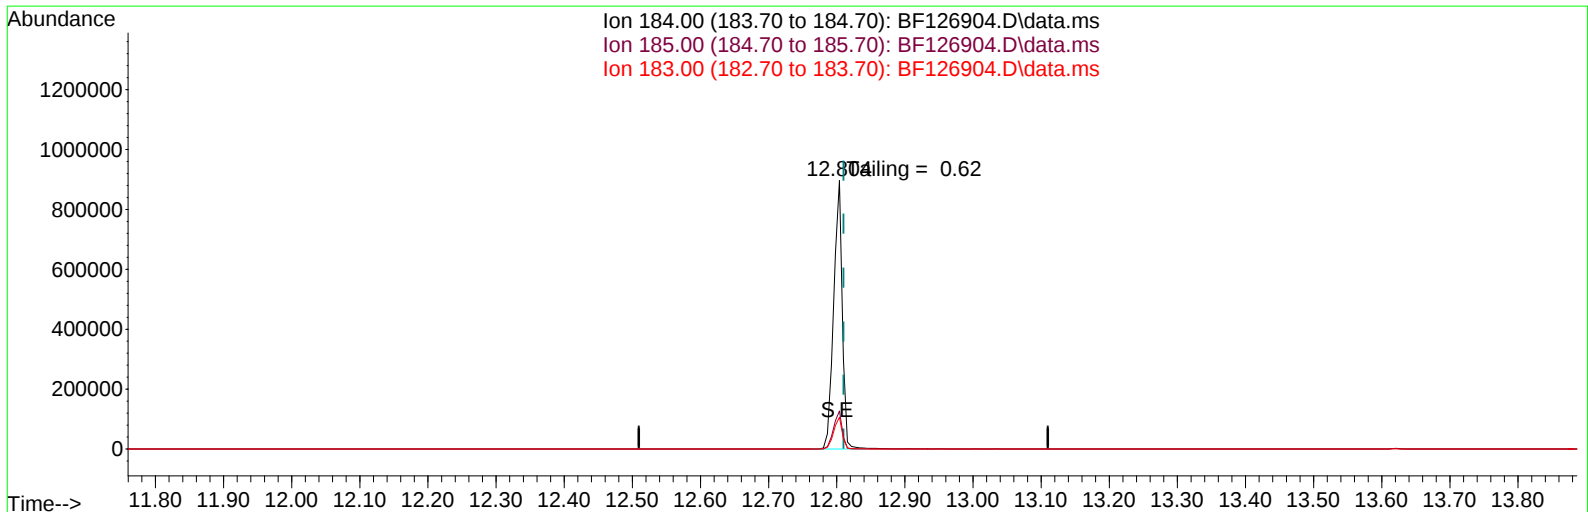

TIC: BF126904.D\data.ms

(77) Benzidine

12.804min (-0.006) 0.00 ng

response 791164

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.60	14.19
183.00	12.00	11.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2022	BNA_F	<u>BF126904.D</u>
Compound Name	Response	Retention Time
DDT	361229	13.62
DDD	3652	13.31
DDE	133	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3785	365014	1.04

Instrument :
BNA_F
ClientSampleId :
DFTPP