
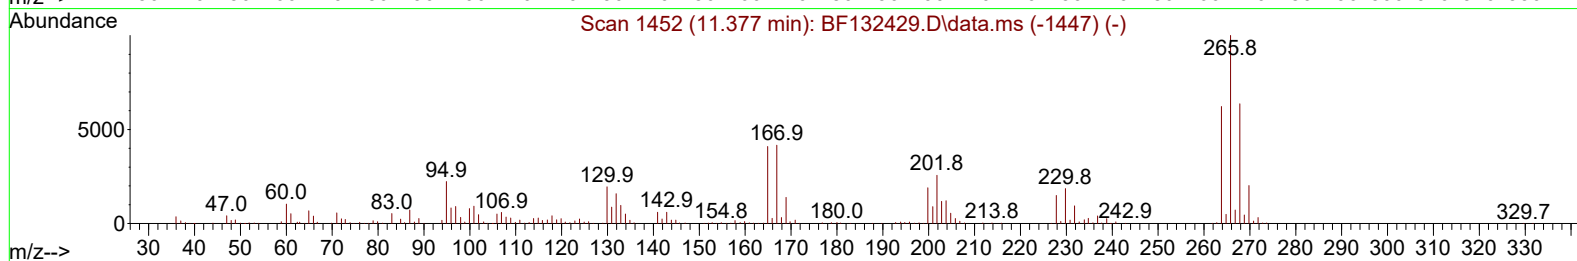
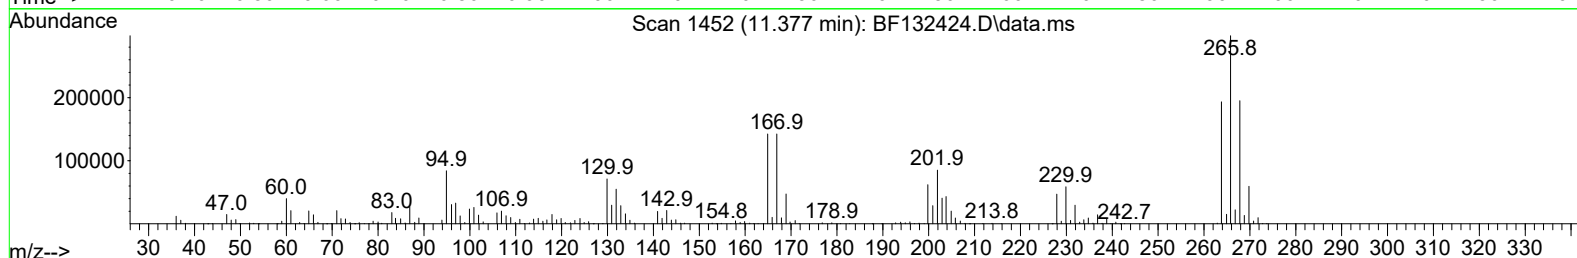


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021623\
 Data File : BF132424.D
 Acq On : 16 Feb 2023 09:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 07:21:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 03:08:40 2023
 Response via : Initial Calibration

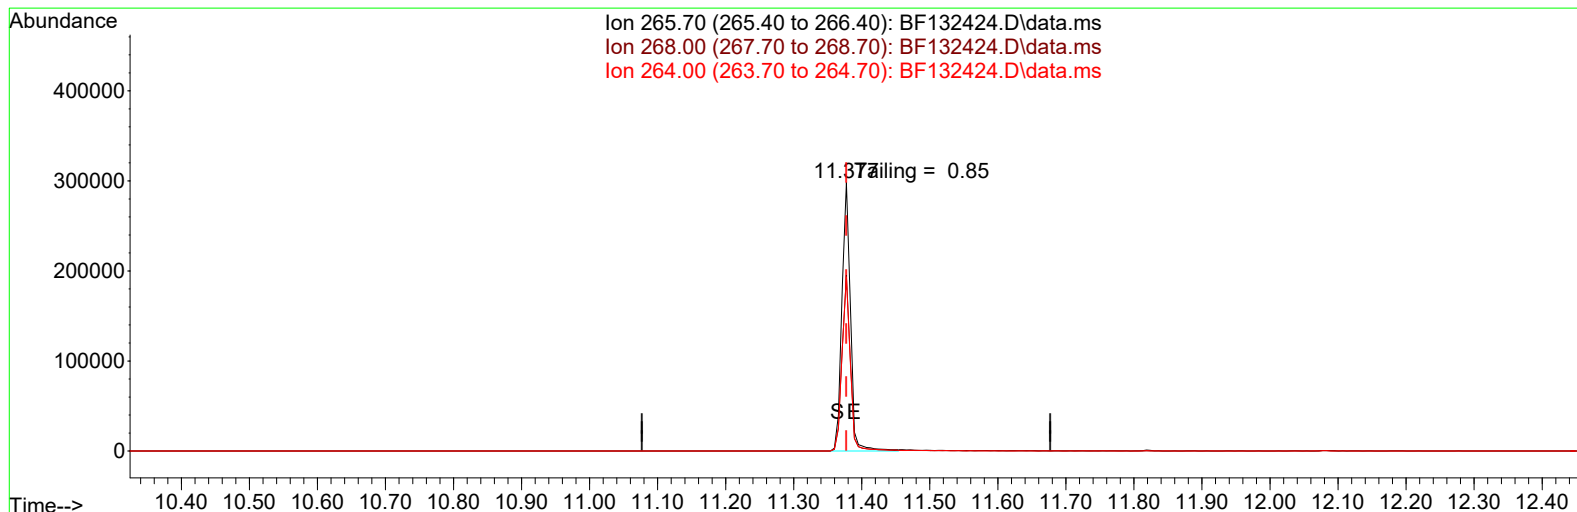

TIC: BF132424.D\data.ms

(70) Pentachlorophenol (C)




11.377min (+ 0.000) 471306.00 ng

response 261848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.46
264.00	62.20	64.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021623\
Data File : BF132424.D
Acq On : 16 Feb 2023 09:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 07:21:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 03:08:40 2023
Response via : Initial Calibration

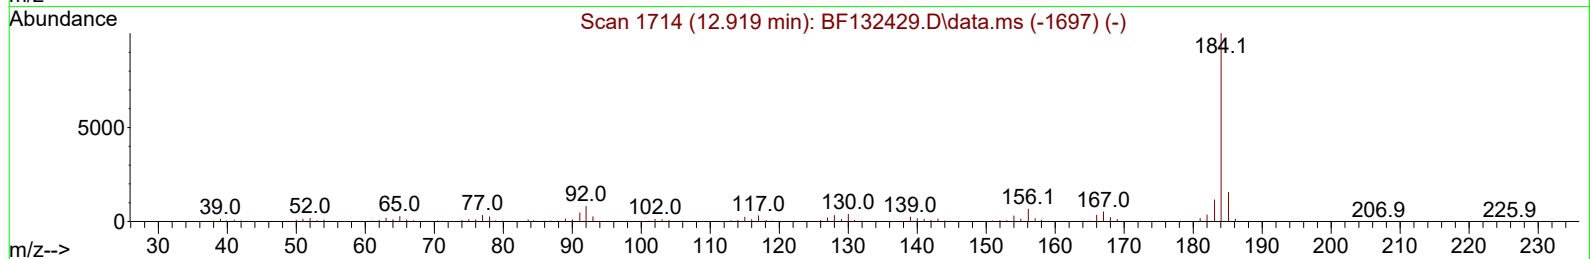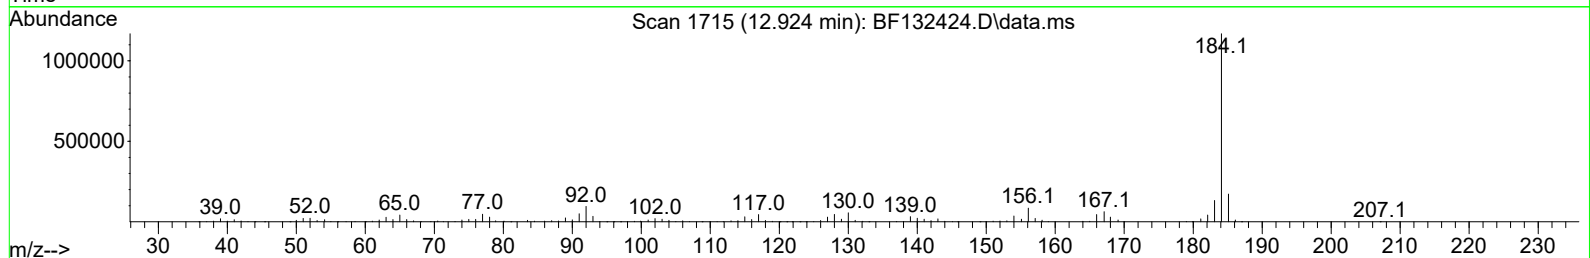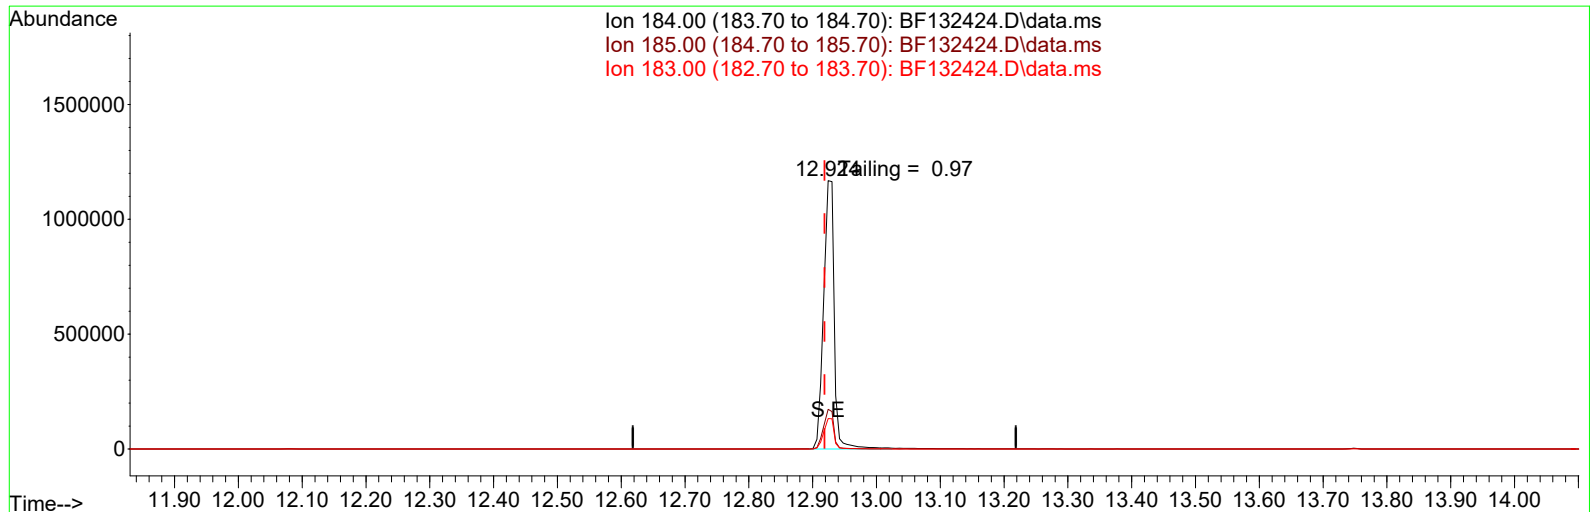

TIC: BF132424.D\data.ms

(77) Benzidine**12.924min (+ 0.006) 44739.01 ng****response 1364216**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	11.50	11.34
0.00	0.00	0.00