


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021623\
 Data File : BF132424.D
 Acq On : 16 Feb 2023 09:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 03:08:40 2023

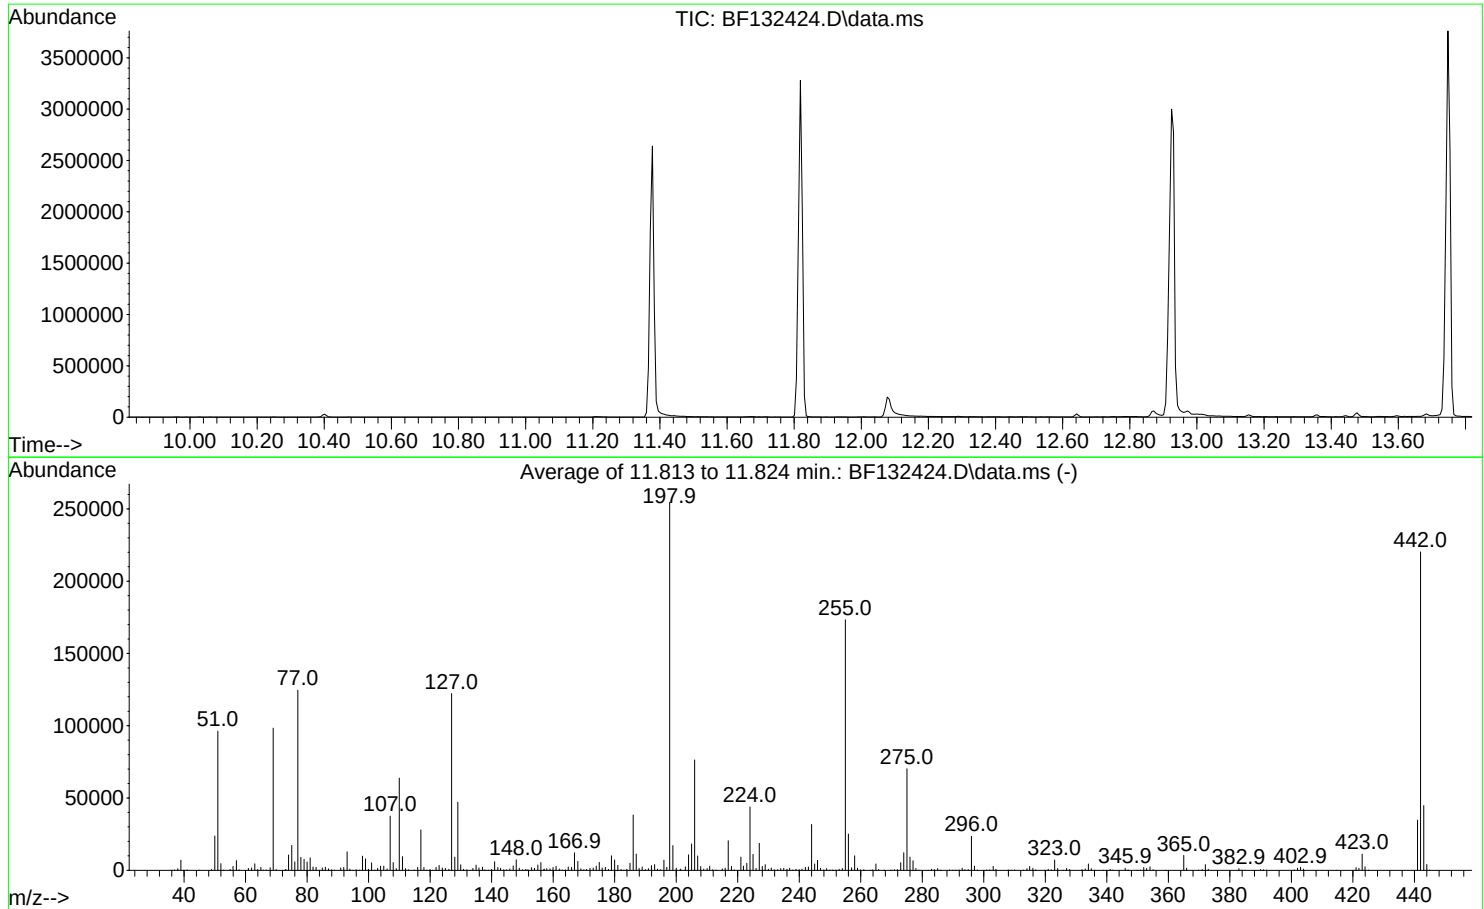




AutoFind: Scans 1526, 1527, 1528; Background Corrected with Scan 1521

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.8	96251	PASS
68	69	0.00	2	1.8	1811	PASS
69	198	0.00	100	38.6	98347	PASS
70	69	0.00	2	0.5	506	PASS
127	198	10	80	48.0	122248	PASS
197	198	0.00	2	0.8	2005	PASS
198	198	100	100	100.0	254485	PASS
199	198	5	9	6.7	17060	PASS
275	198	10	60	27.6	70200	PASS
365	198	1	100	4.1	10348	PASS
441	198	0.01	100	13.6	34689	PASS
442	442	50	100	100.0	220267	PASS
443	442	15	24	20.3	44776	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021623\
 Data File : BF132424.D
 Acq On : 16 Feb 2023 09:39
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 17 07:21:39 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 03:08:40 2023
 Response via : Initial Calibration

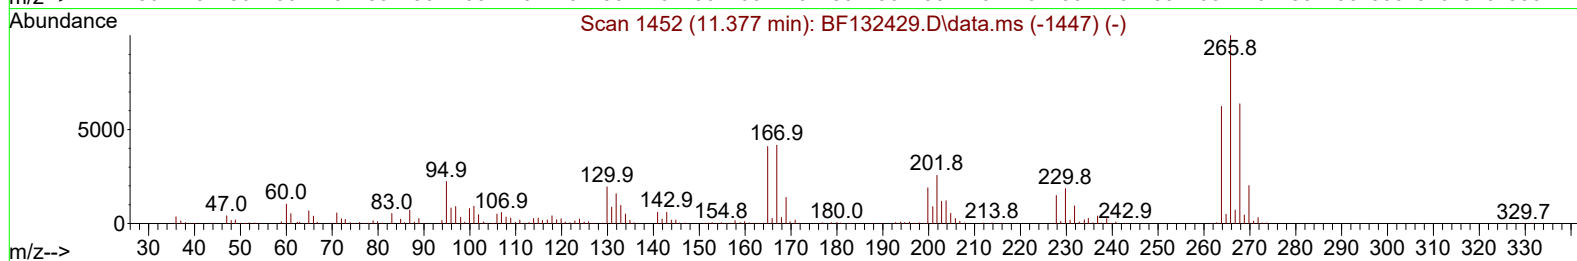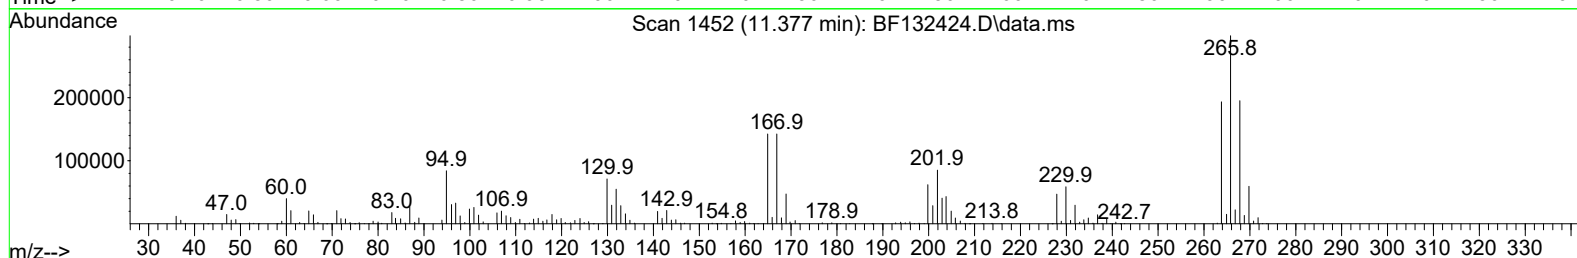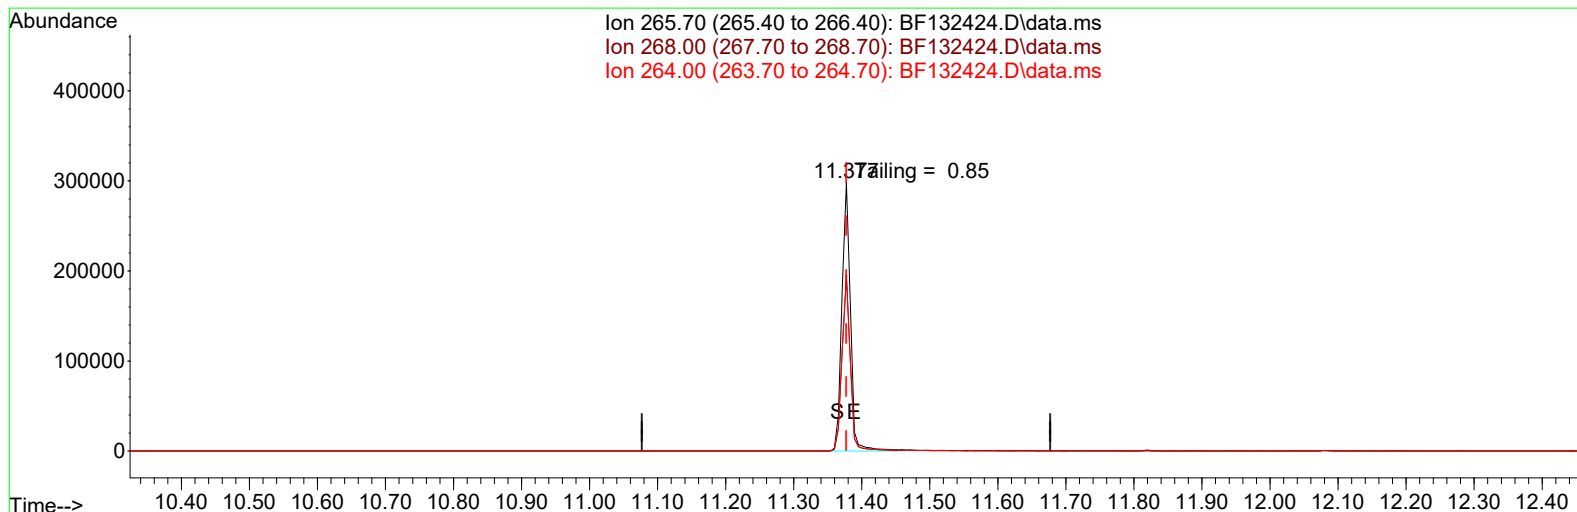

TIC: BF132424.D\data.ms

(70) Pentachlorophenol (C)

11.377min (+ 0.000) 471306.00 ng




response 261848

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.70	65.46
264.00	62.20	64.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021623\
Data File : BF132424.D
Acq On : 16 Feb 2023 09:39
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 17 07:21:39 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 03:08:40 2023
Response via : Initial Calibration

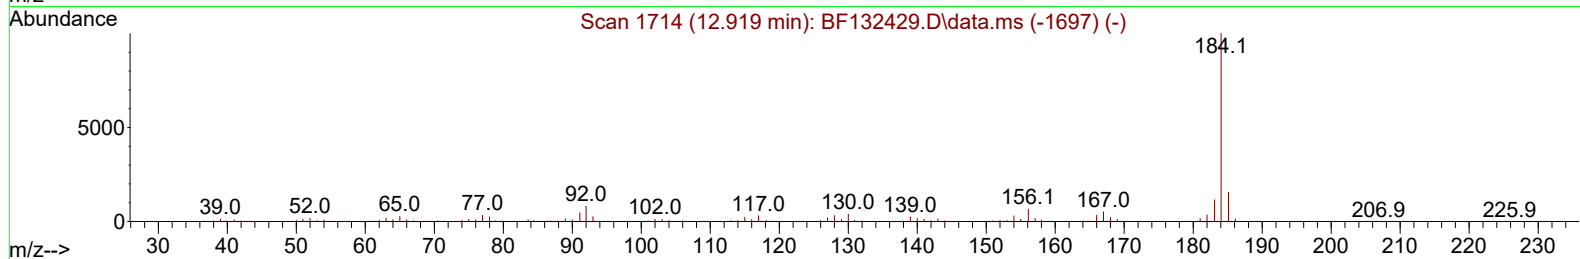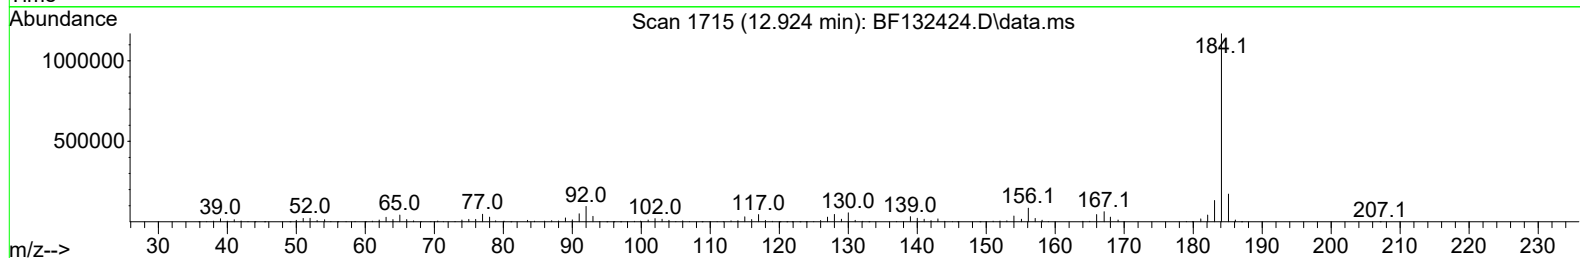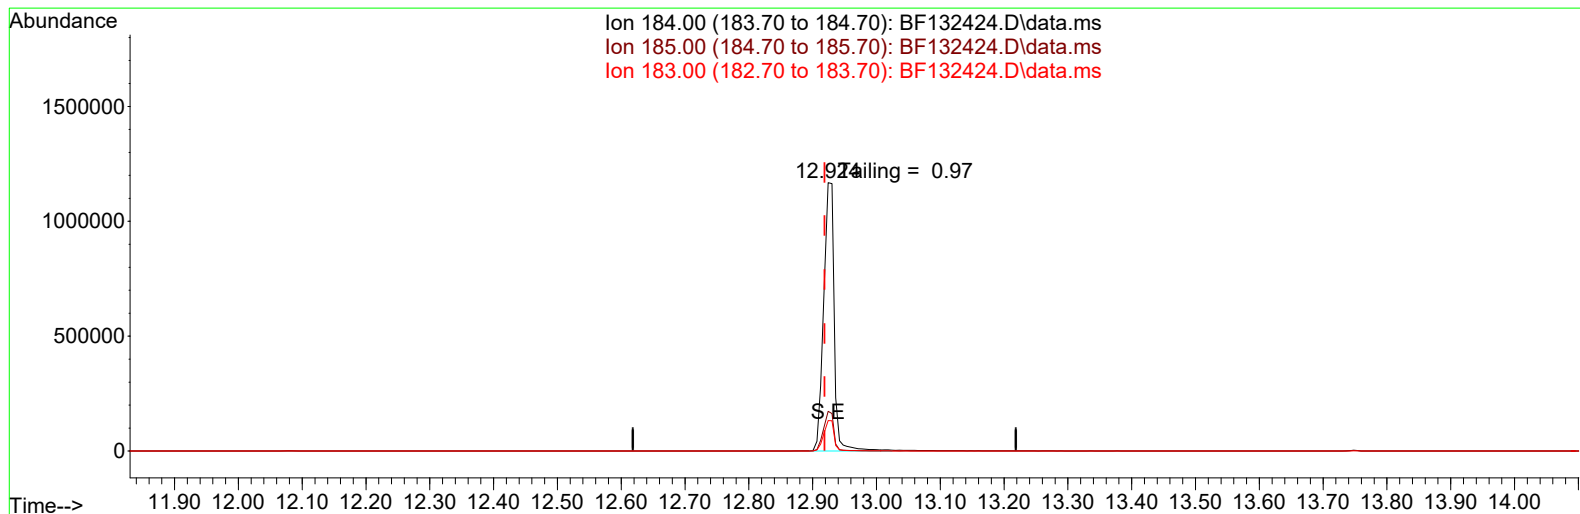

TIC: BF132424.D\data.ms

(77) Benzidine

12.924min (+ 0.006) 44739.01 ng

response 1364216

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.78
183.00	11.50	11.34
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/16/2023	BNA_F	<u>BF132424.D</u>
Compound Name	Response	Retention Time
DDT	637038	13.748
DDD	7469	13.477
DDE	57	13.154
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7526	644564	1.17

Instrument :
BNA_F
ClientSampleId :
DFTPP