


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021715\
 Data File : BF077319.D
 Acq On : 17 Feb 2015 16:40
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 18 02:50:27 2015

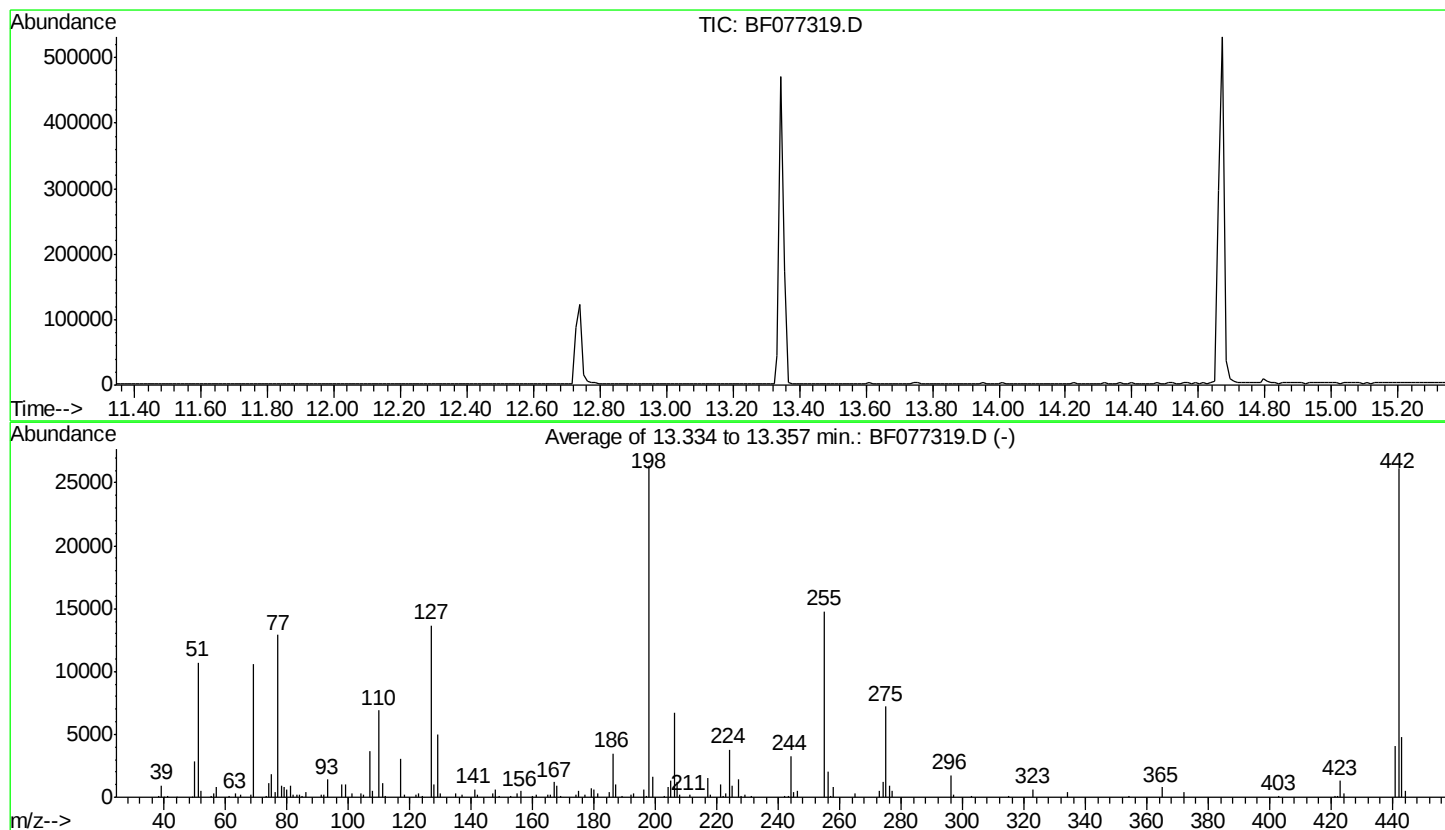

AutoFind: Scans 1089, 1090, 1091; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.7	10736	PASS
68	69	0.00	2	1.5	157	PASS
69	198	0.00	100	40.2	10613	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.8	13651	PASS
197	198	0.00	2	0.4	111	PASS
198	198	100	100	100.0	26370	PASS
199	198	5	9	6.3	1653	PASS
275	198	10	60	27.3	7199	PASS
365	198	1	100	3.1	806	PASS
441	442	0.01	24	15.7	4094	PASS
442	198	50	100	99.1	26130	PASS
443	442	15	24	18.3	4781	PASS