


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021715\
 Data File : BF077328.D
 Acq On : 17 Feb 2015 21:26
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Feb 18 02:50:27 2015

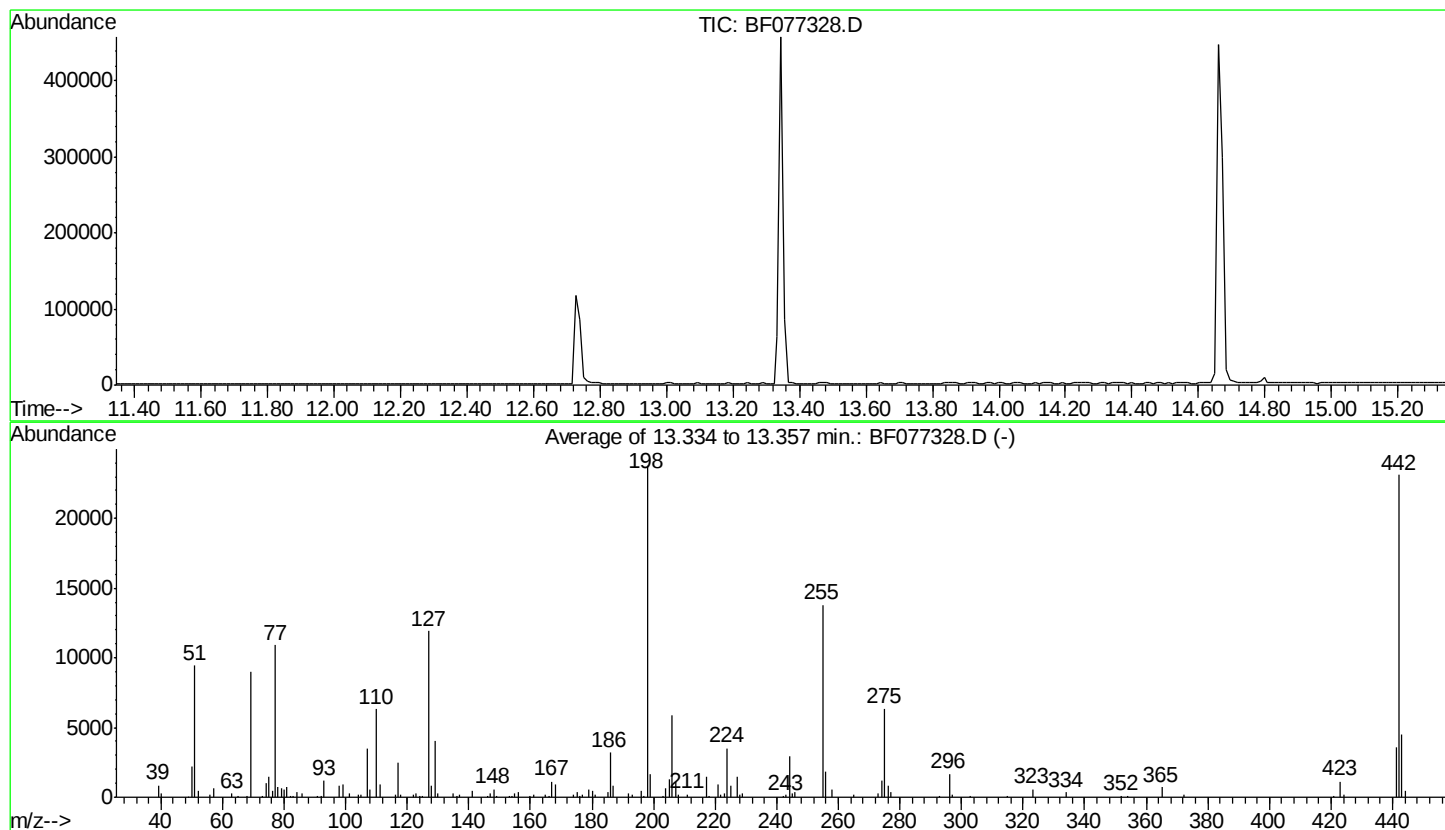

AutoFind: Scans 1089, 1090, 1091; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	9436	PASS
68	69	0.00	2	1.3	113	PASS
69	198	0.00	100	37.7	8963	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.0	11905	PASS
197	198	0.00	2	0.5	128	PASS
198	198	100	100	100.0	23787	PASS
199	198	5	9	6.9	1651	PASS
275	198	10	60	26.7	6346	PASS
365	198	1	100	2.9	701	PASS
441	442	0.01	24	15.4	3566	PASS
442	198	50	100	97.2	23128	PASS
443	442	15	24	19.4	4486	PASS