
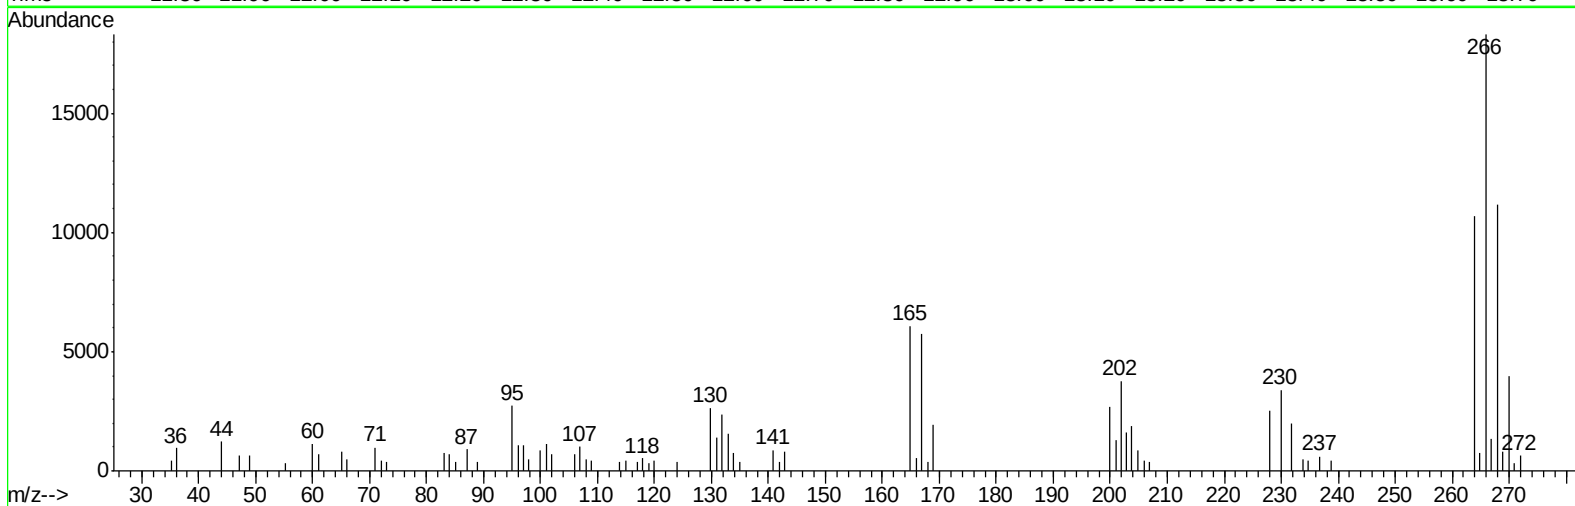


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021715\
Data File : BF077319.D
Acq On : 17 Feb 2015 16:40
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 07:05:06 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 02:50:27 2015
Response via : Initial Calibration

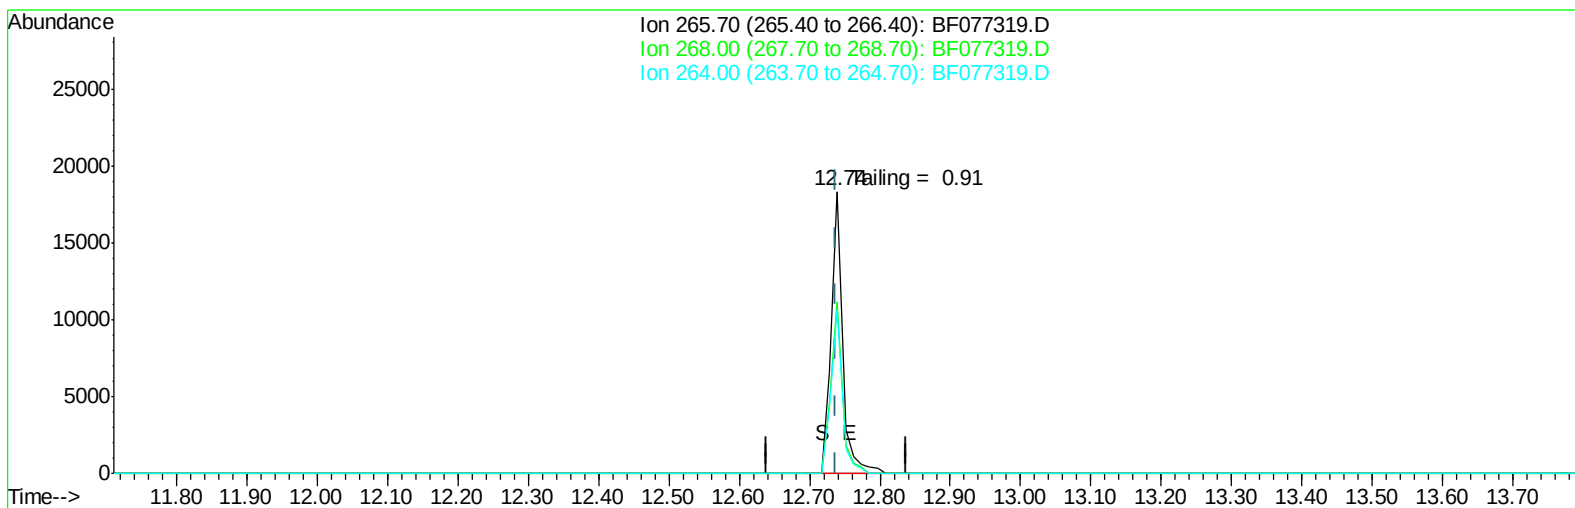

TIC: BF077319.D

(69) Pentachlorophenol (C)



12.739min (+0.000) 0.00ng

response 20684

Ion	Exp%	Act%
265.70	100	100
268.00	67.50	61.09
264.00	60.20	58.26
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021715\
Data File : BF077319.D
Acq On : 17 Feb 2015 16:40
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 07:05:06 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 02:50:27 2015
Response via : Initial Calibration

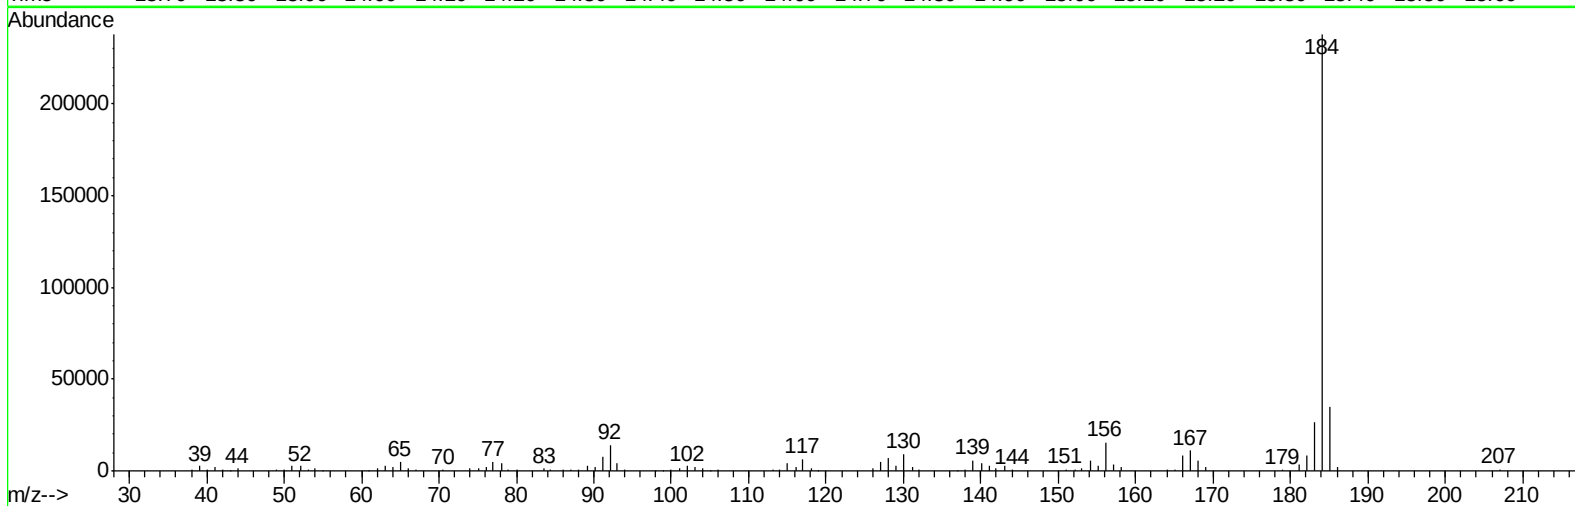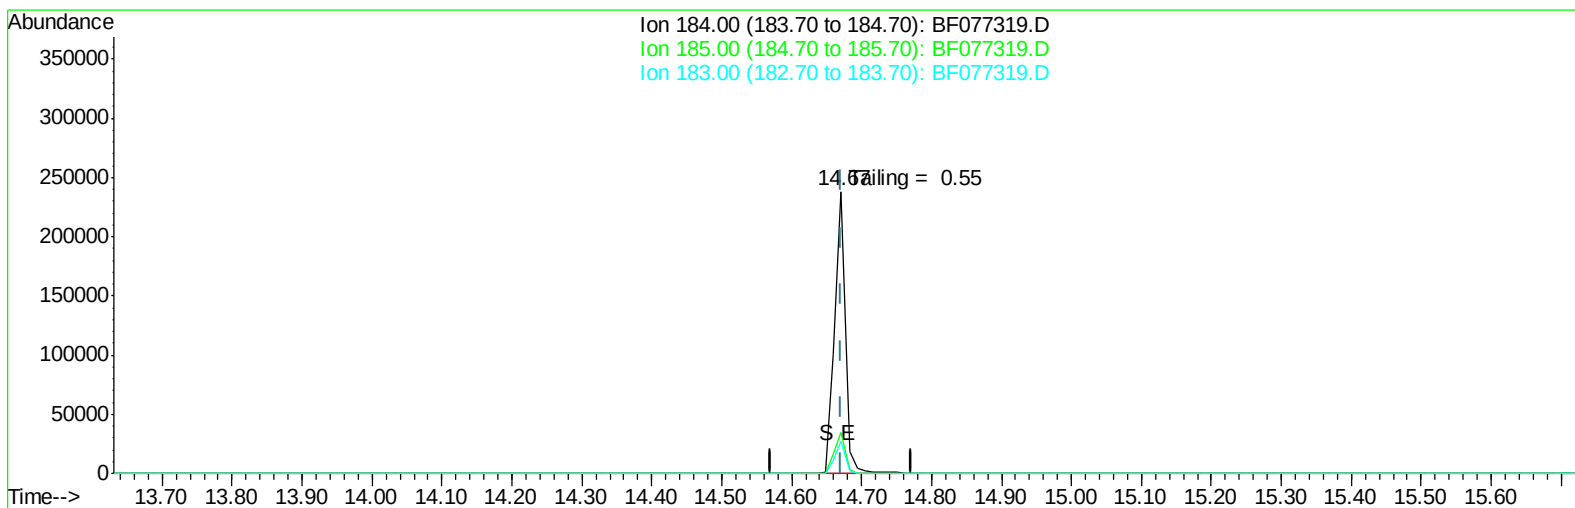

TIC: BF077319.D

(76) Benzidine

14.671min (-0.000) 0.00ng

response 251129

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.75
183.00	11.60	11.23
0.00	0.00	0.00