
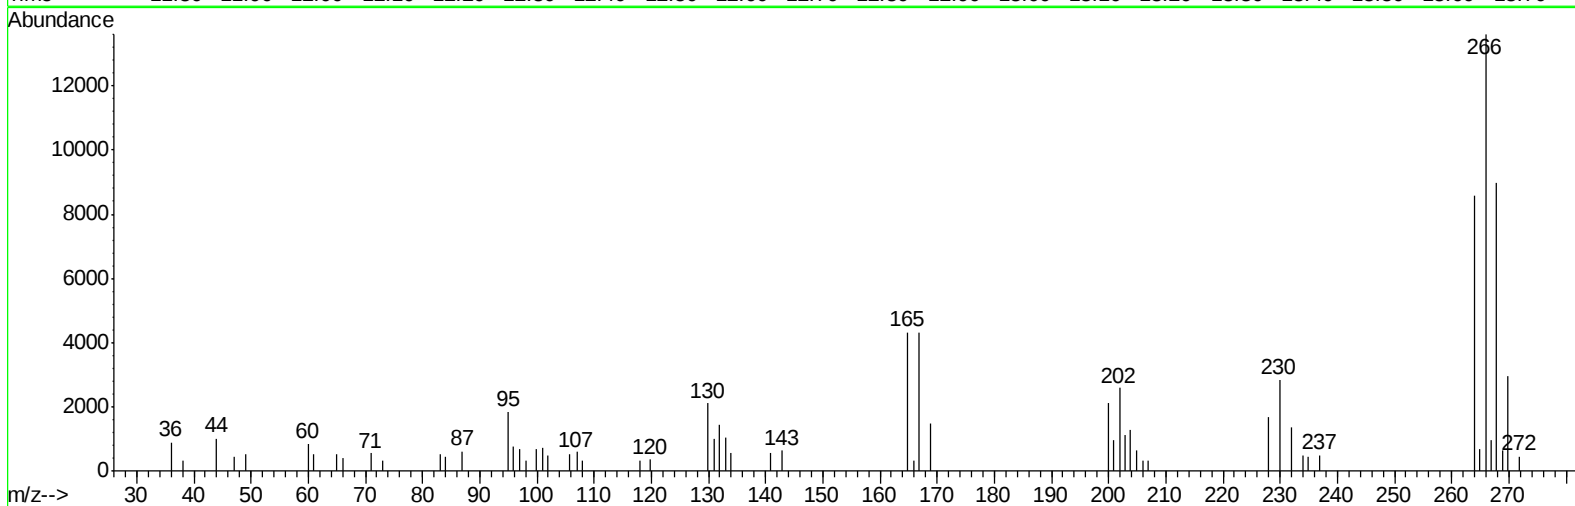


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021715\
Data File : BF077328.D
Acq On : 17 Feb 2015 21:26
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 07:09:43 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 02:50:27 2015
Response via : Initial Calibration

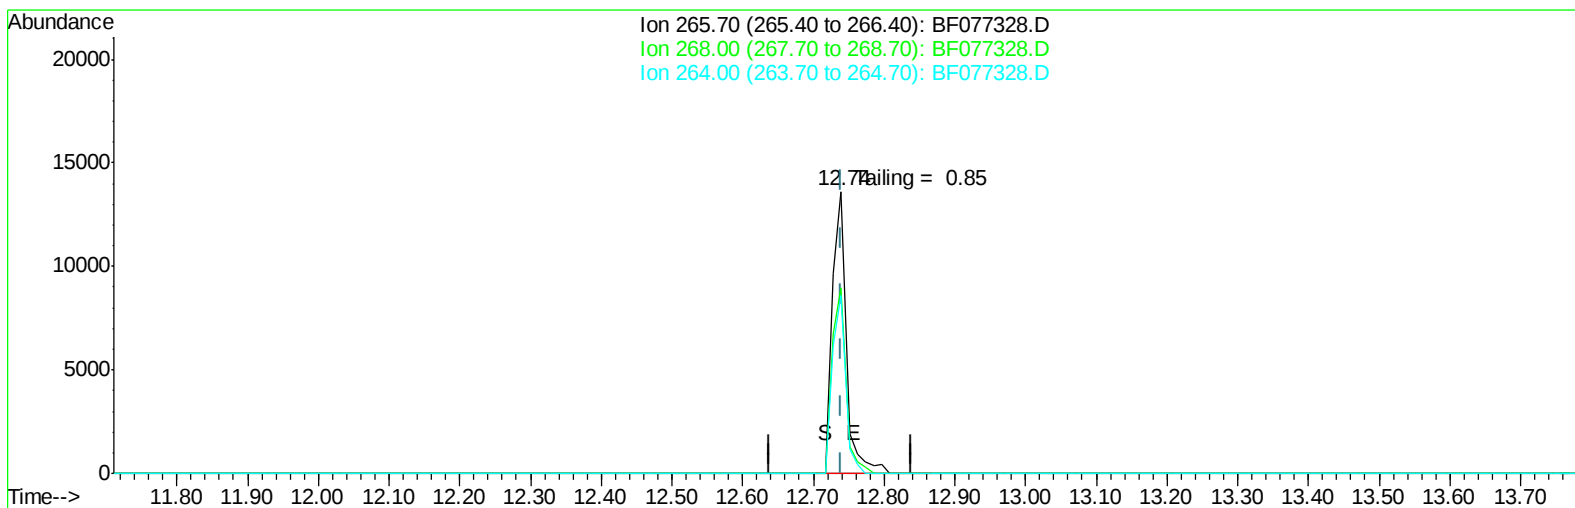

TIC: BF077328.D

(69) Pentachlorophenol (C)



12.740min (+0.000) 0.00ng

response 18575

Ion	Exp%	Act%
265.70	100	100
268.00	67.50	65.86
264.00	60.20	63.00
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021715\
Data File : BF077328.D
Acq On : 17 Feb 2015 21:26
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 07:09:43 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 02:50:27 2015
Response via : Initial Calibration

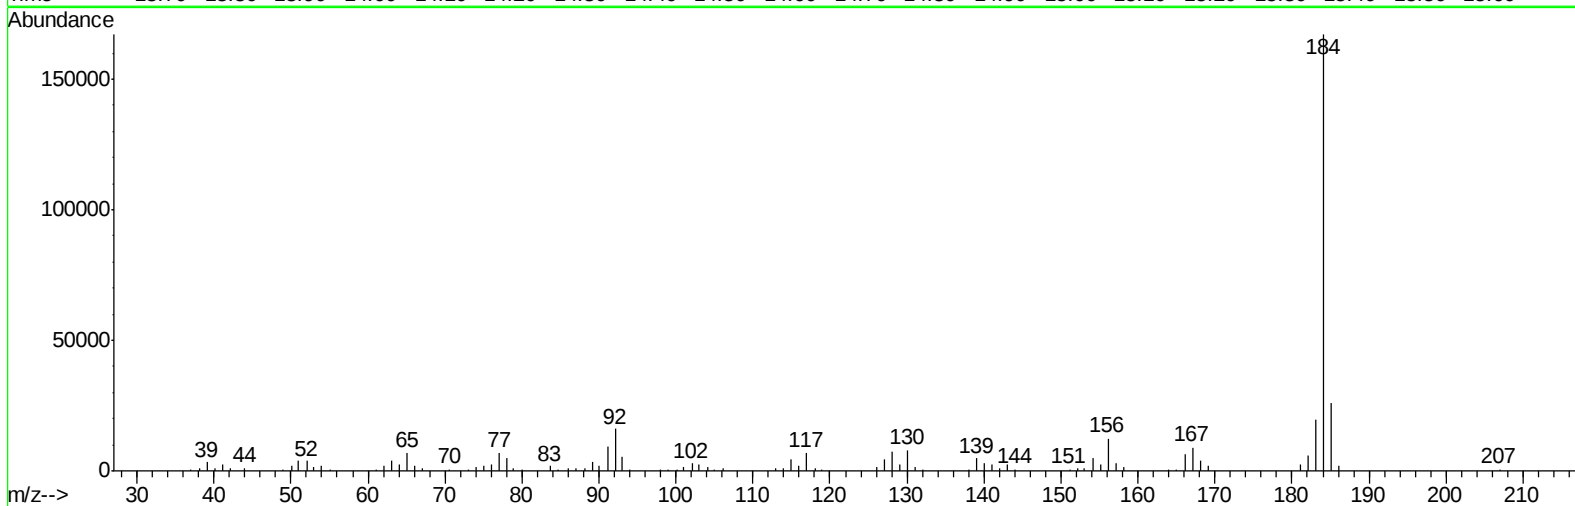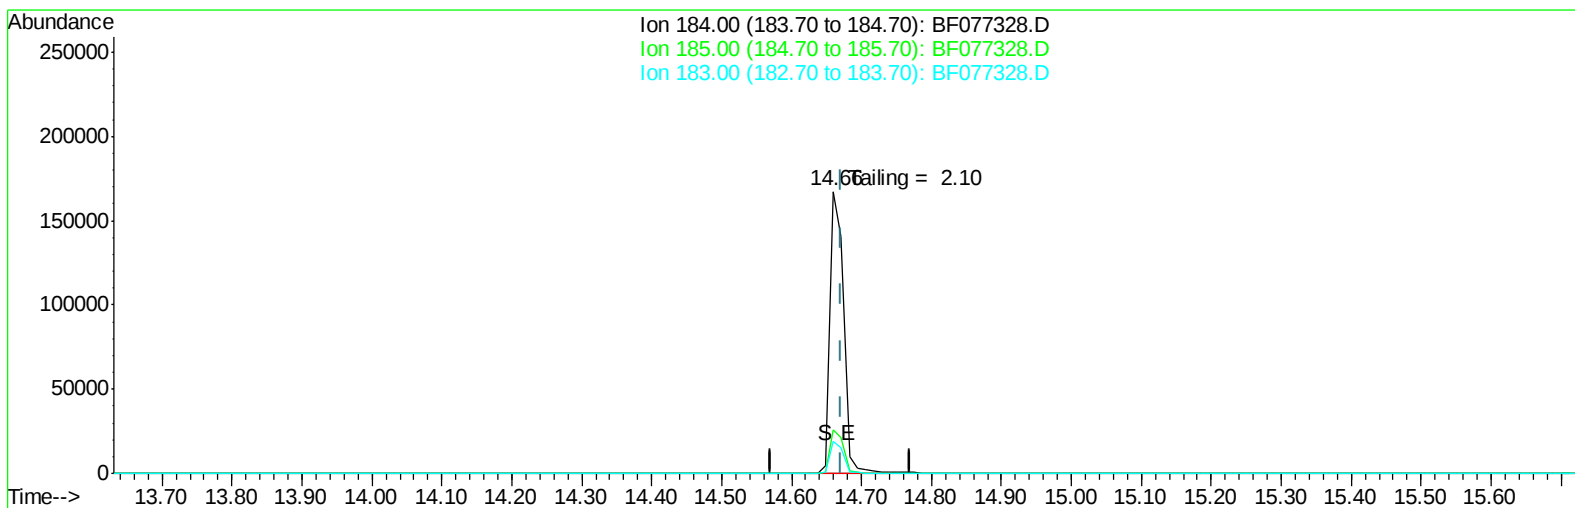

TIC: BF077328.D

(76) Benzidine

14.660min (-0.011) 0.00ng

response 225969

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	15.50
183.00	11.60	11.60
0.00	0.00	0.00