


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021715\
Data File : BF077328.D
Acq On : 17 Feb 2015 21:54
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Feb 18 09:51:00 2015

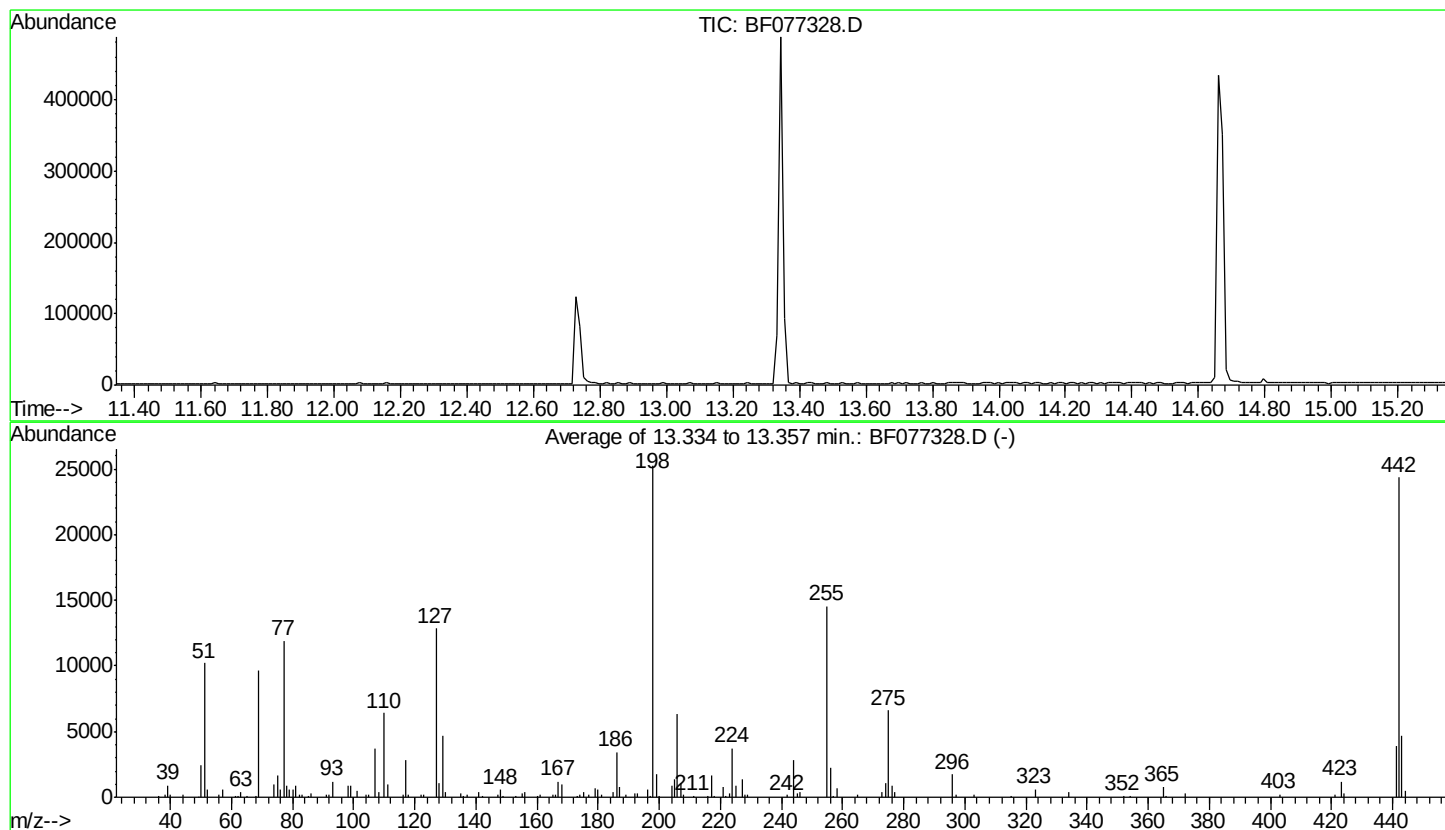

AutoFind: Scans 1089, 1090, 1091; Background Corrected with Scan 1086

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	10211	PASS
68	69	0.00	2	1.3	126	PASS
69	198	0.00	100	38.4	9704	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	12841	PASS
197	198	0.00	2	0.4	102	PASS
198	198	100	100	100.0	25264	PASS
199	198	5	9	7.0	1757	PASS
275	198	10	60	26.2	6627	PASS
365	198	1	100	3.2	805	PASS
441	442	0.01	24	16.0	3910	PASS
442	198	50	100	96.5	24376	PASS
443	442	15	24	19.3	4699	PASS