
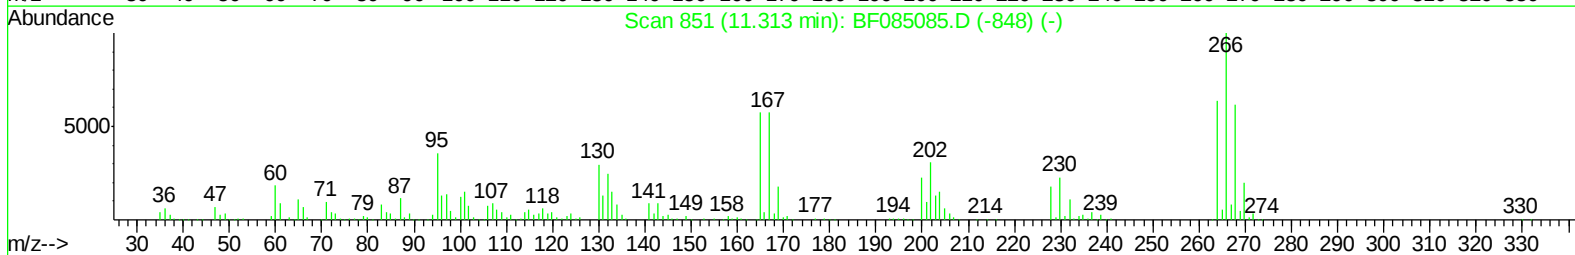
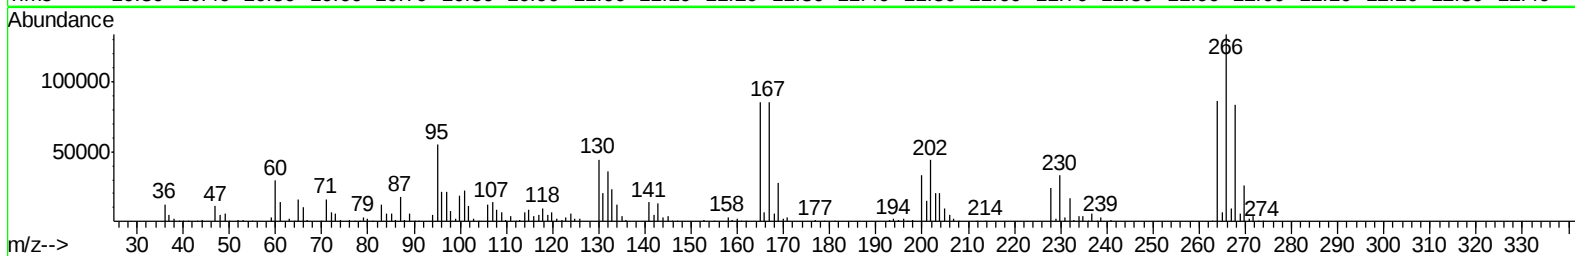


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021716\
Data File : BF085081.D
Acq On : 17 Feb 2016 9:43
Operator : SJ/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:53:58 2016
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021716.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 17 16:42:47 2016
Response via : Initial Calibration

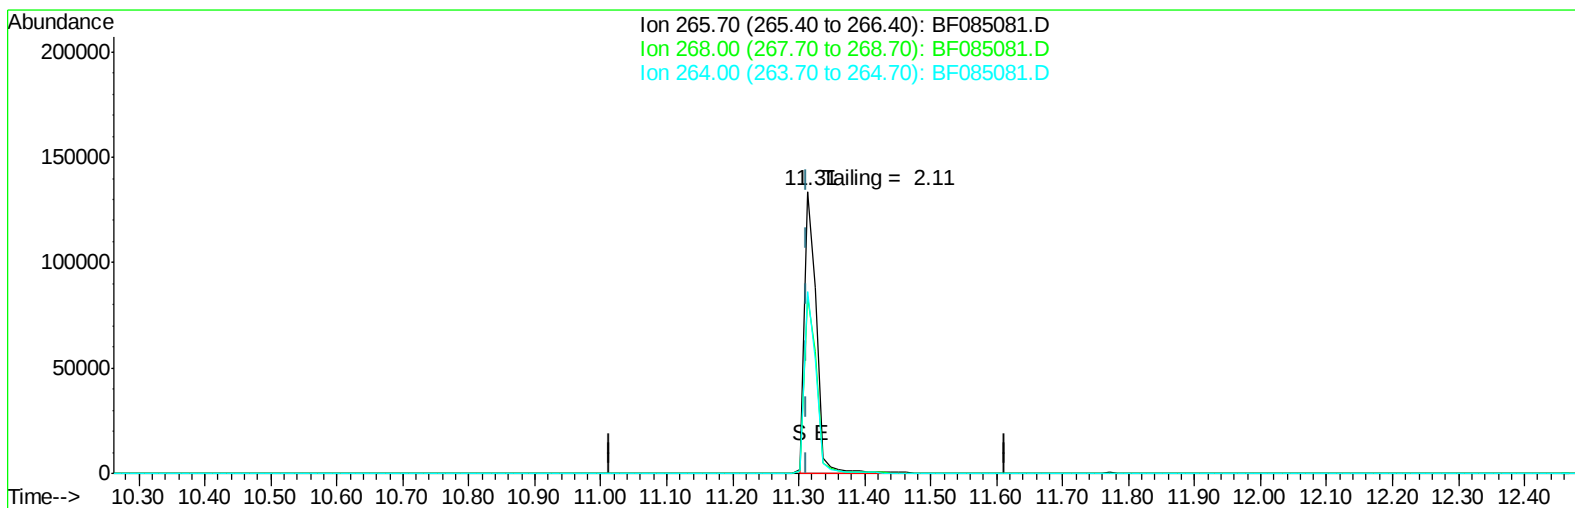

TIC: BF085081.D

(69) Pentachlorophenol (C)




11.314min (+0.000) 29886.34ng

response 166821

Ion	Exp%	Act%
265.70	100	100
268.00	59.10	62.69
264.00	62.20	64.43
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021716\
 Data File : BF085081.D
 Acq On : 17 Feb 2016 9:43
 Operator : SJ/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:53:58 2016
 Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF021716.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 17 16:42:47 2016
 Response via : Initial Calibration

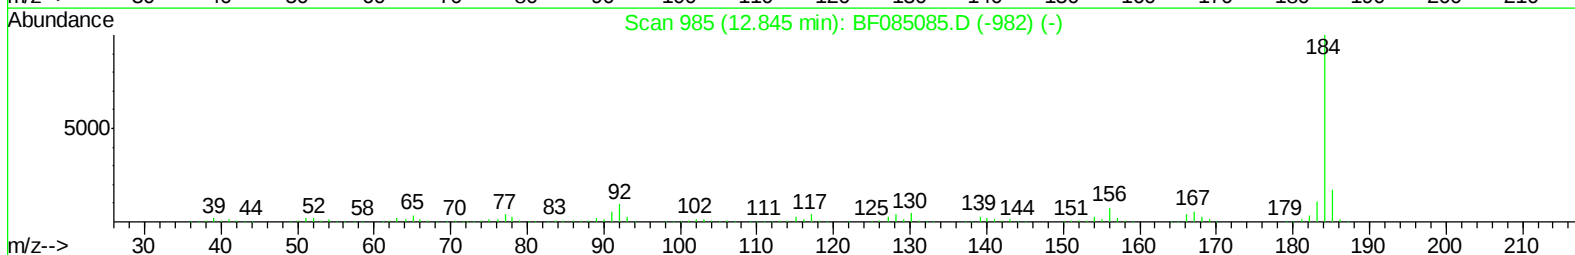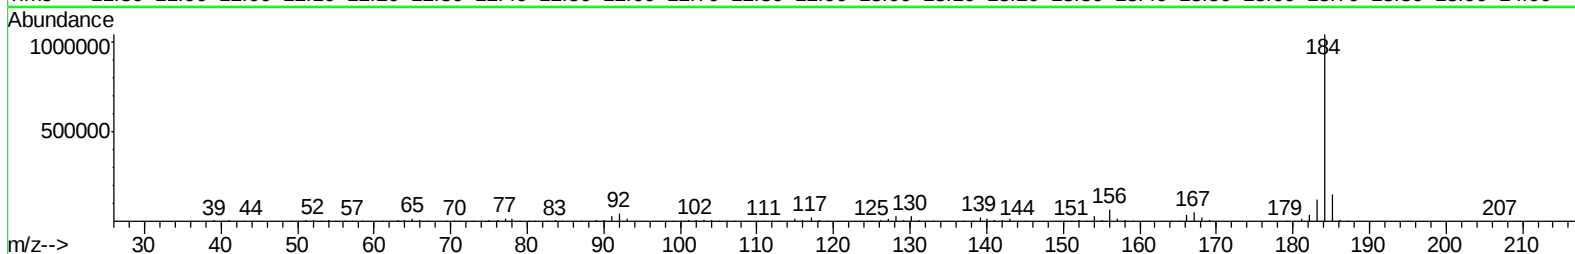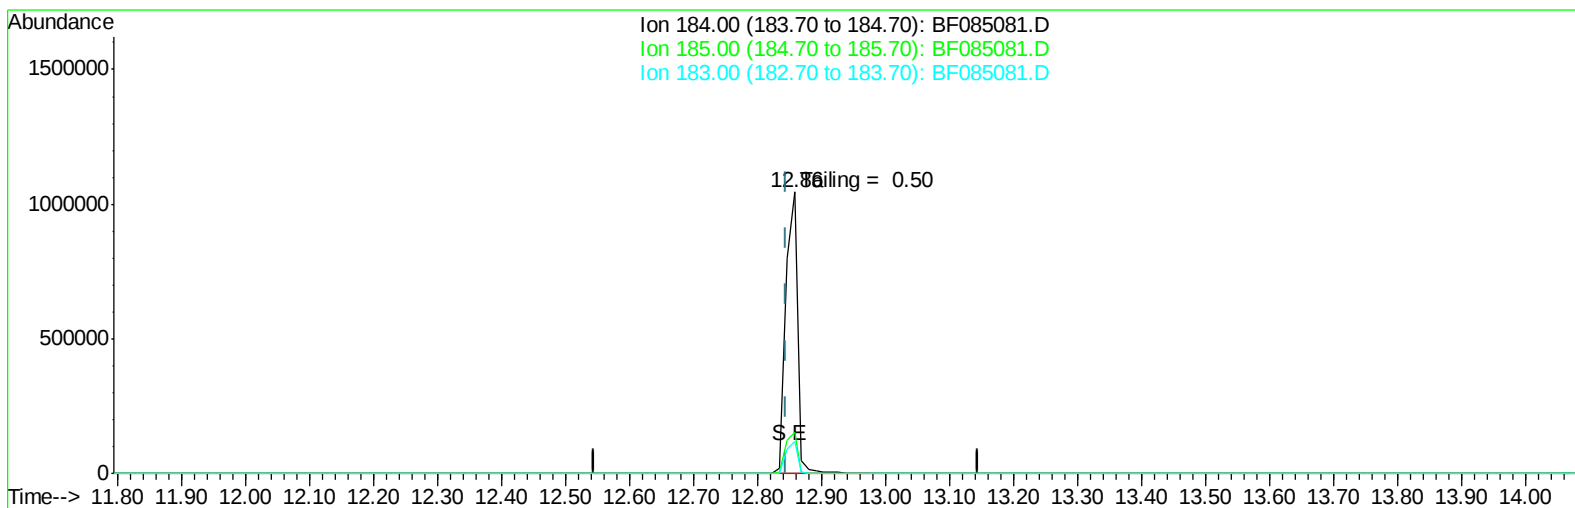

TIC: BF085081.D

(76) Benzidine

12.857min (+0.012) 147063.84ng

response 1350853

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.60
183.00	10.70	11.40
0.00	0.00	0.00