
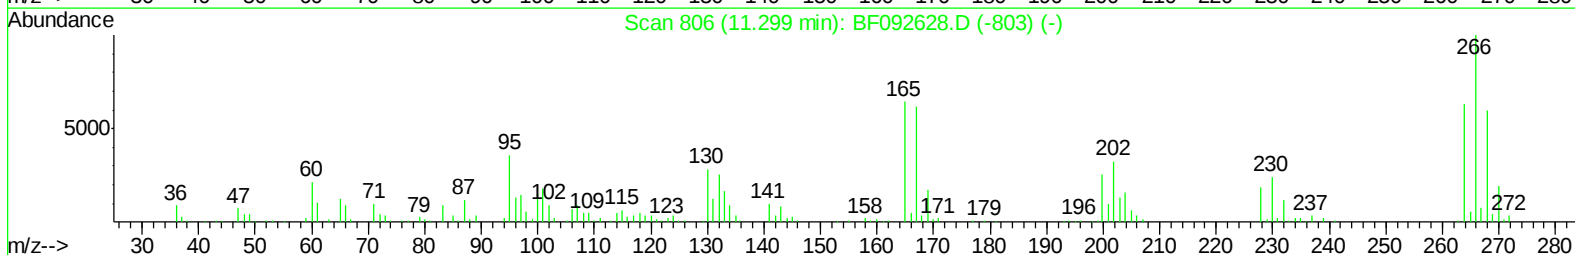
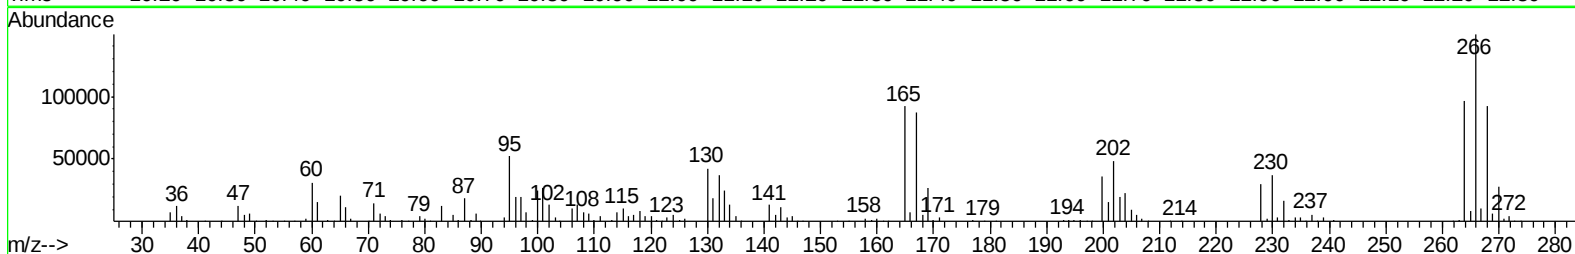


Data File : BF093004.D
Acq On : 17 Feb 2017 12:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 00:39:36 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

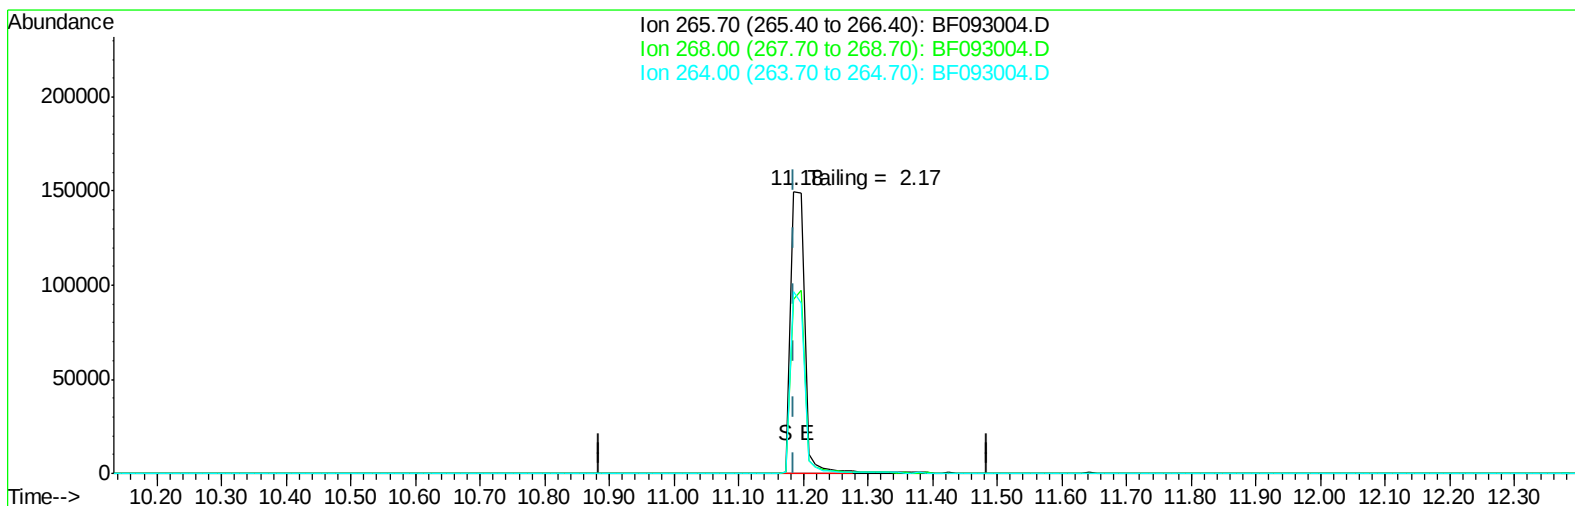

TIC: BF093004.D

(69) Pentachlorophenol (C)




11.185min (-0.000) 0.00ng

response 226845

Ion	Exp%	Act%
265.70	100	100
268.00	66.60	61.95
264.00	62.90	64.55
0.00	0.00	0.00

Data File : BF093004.D
Acq On : 17 Feb 2017 12:11
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 00:39:36 2017
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 17:31:55 2017
Response via : Initial Calibration

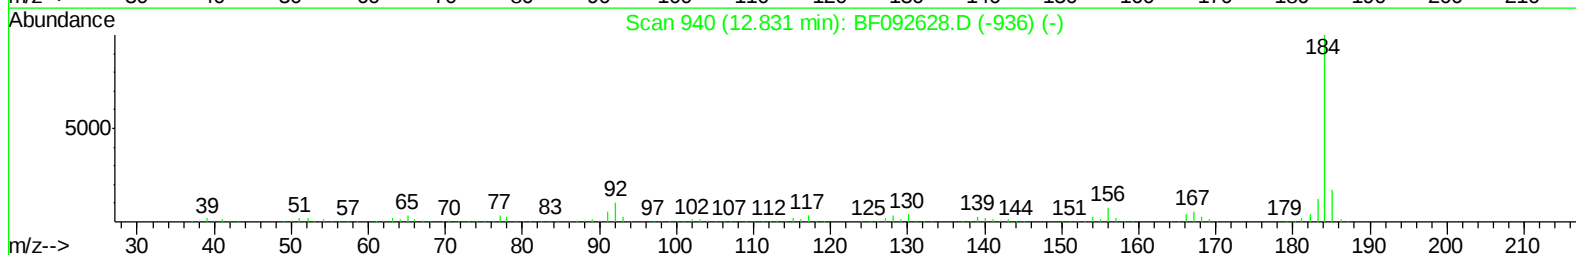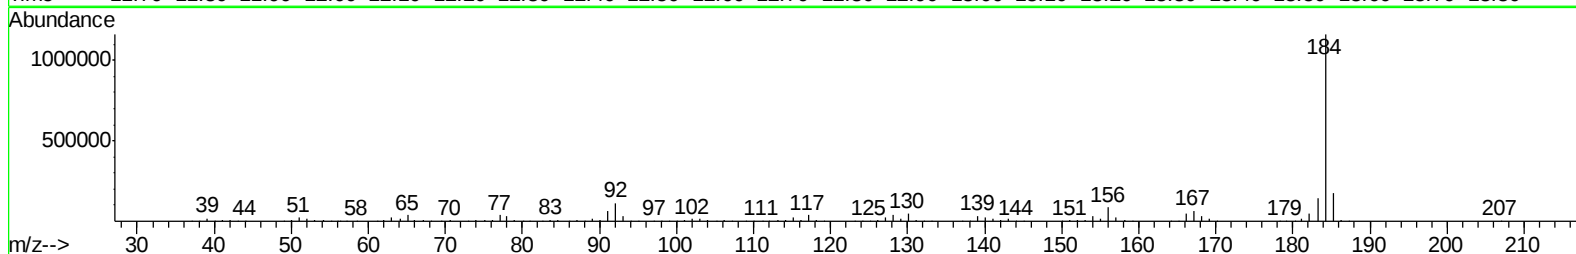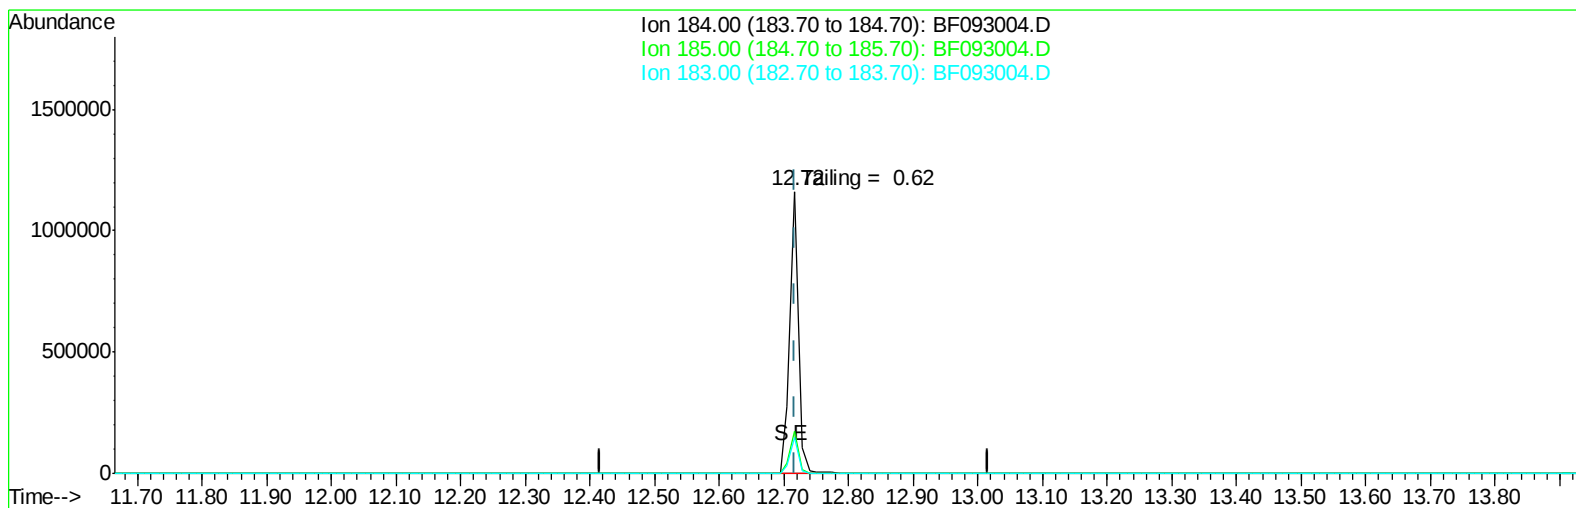

TIC: BF093004.D

(76) Benzidine

12.716min (-0.000) 44737.42ng

response 1084732

Ion	Exp%	Act%
184.00	100	100
185.00	16.70	14.84
183.00	11.50	12.72
0.00	0.00	0.00