


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021717\
 Data File : BF093004.D
 Acq On : 17 Feb 2017 12:11
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF013017.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 17 17:31:55 2017

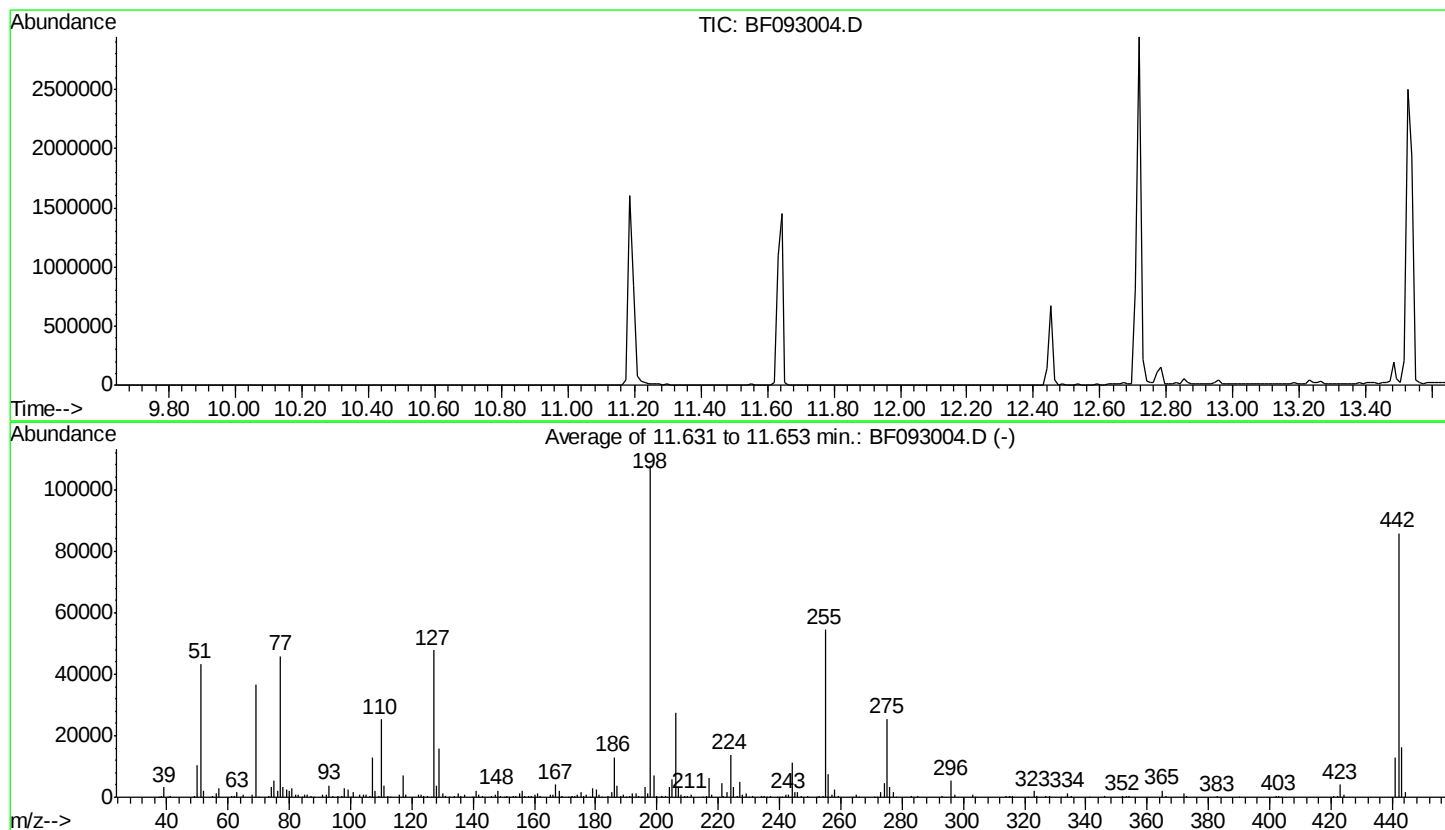

AutoFind: Scans 835, 836, 837; Background Corrected with Scan 831

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	43283	PASS
68	69	0.00	2	1.8	670	PASS
69	198	0.00	100	33.8	36489	PASS
70	69	0.00	2	0.3	101	PASS
127	198	10	80	44.3	47722	PASS
197	198	0.00	2	1.2	1309	PASS
198	198	100	100	100.0	107801	PASS
199	198	5	9	6.4	6899	PASS
275	198	10	60	23.6	25415	PASS
365	198	1	100	2.1	2238	PASS
441	442	0.01	24	15.2	13079	PASS
442	198	50	100	79.6	85823	PASS
443	442	15	24	19.0	16346	PASS