
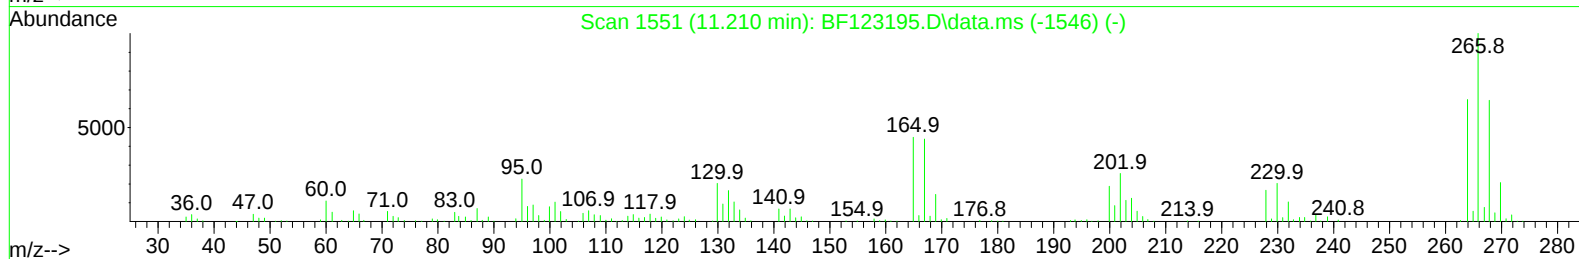
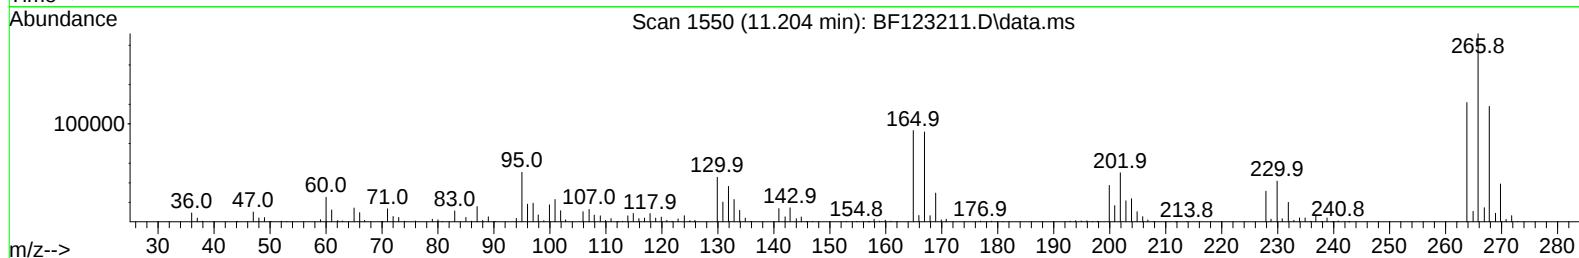


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
Data File : BF123211.D
Acq On : 17 Feb 2021 12:43
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 16:12:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

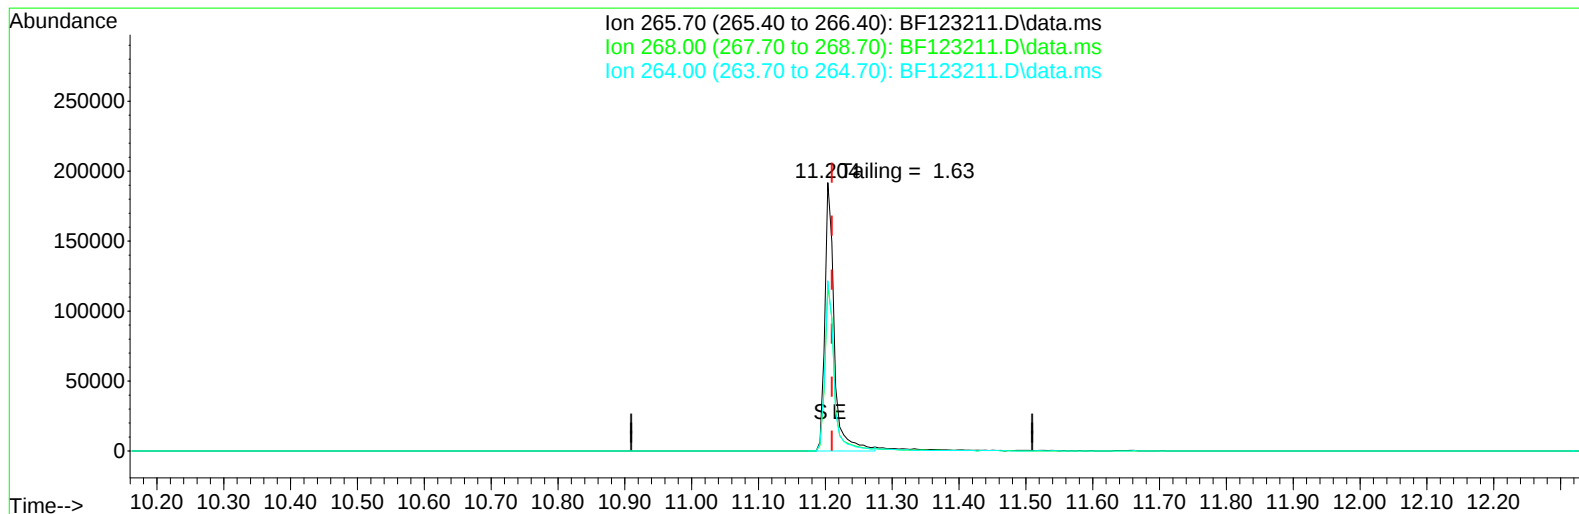

TIC: BF123211.D\data.ms




(70) Pentachlorophenol (C)

11.204min (-0.006) 29045.70 ng

response 192347

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.40
264.00	62.30	63.46
0.00	0.00	0.00

Quant Time: Feb 17 16:12:18 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

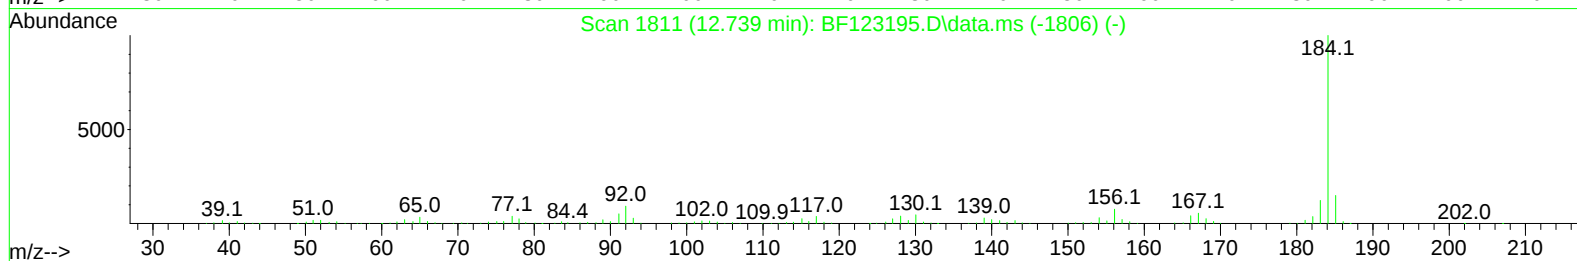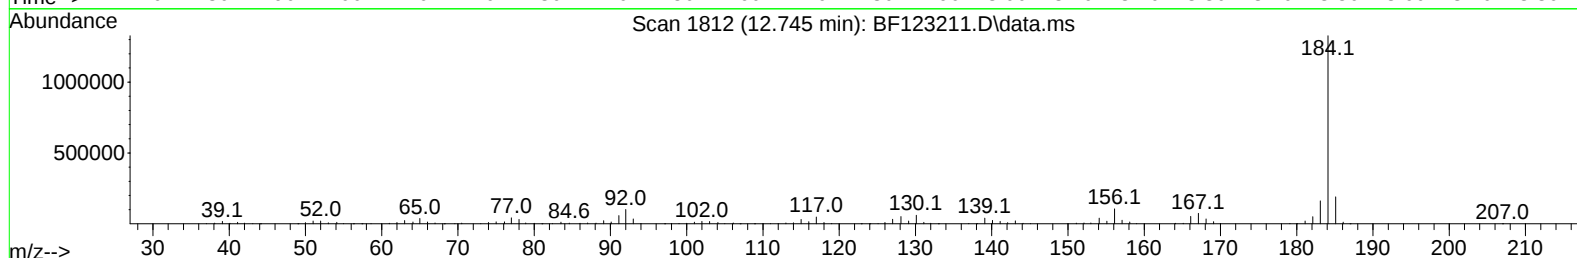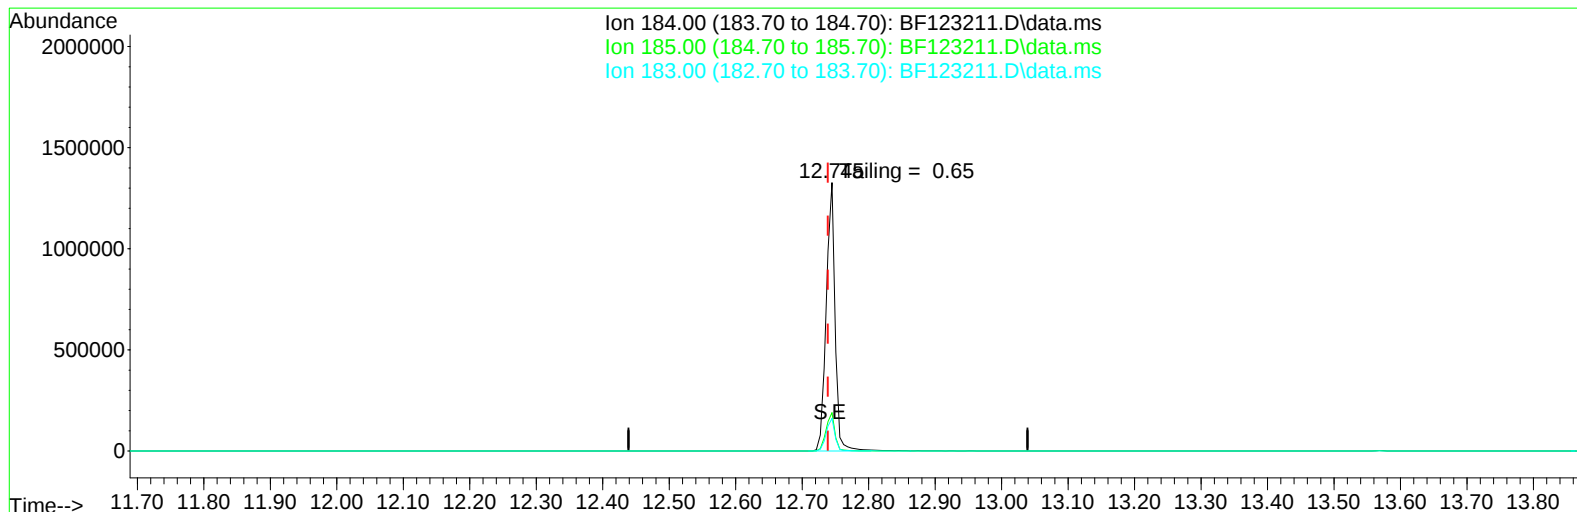

TIC: BF123211.D\data.ms

(77) Benzidine

12.745min (+ 0.006) 0.00 ng

```
response      1234399
```

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.35
183.00	12.10	12.19
0.00	0.00	0.00