

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
 Data File : BF123213.D
 Acq On : 17 Feb 2021 15:24
 Operator : JU/CG
 Sample : PB134684BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134684BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123213.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.281	29	33	42	rVB6	22071	54465	1.06%	0.183%
2	5.492	574	579	582	rBV	4057787	3877266	75.60%	13.061%
3	6.498	744	750	753	rBV	3618551	3820634	74.50%	12.870%
4	6.869	809	813	816	rBV	1007718	803487	15.67%	2.707%
5	7.428	903	908	911	rBV	2345166	2525822	49.25%	8.508%
6	8.151	1026	1031	1035	rBV	1261627	1088614	21.23%	3.667%
7	9.233	1209	1215	1218	rBV	4540716	4535283	88.43%	15.277%
8	9.910	1325	1330	1334	rBV	1384228	1214652	23.68%	4.092%
9	10.704	1459	1465	1468	rBV	2980304	2865335	55.87%	9.652%
10	11.398	1579	1583	1587	rBV	1308241	1247646	24.33%	4.203%
11	11.933	1670	1674	1694	rBV4	81183	246468	4.81%	0.830%
12	12.733	1807	1810	1819	rBV8	20224	57279	1.12%	0.193%
13	12.998	1849	1855	1858	rBV	5431432	5128649	100.00%	17.276%
14	14.051	2030	2034	2039	rBV	1343698	1166245	22.74%	3.928%
15	15.527	2280	2285	2295	rBV	808525	1055027	20.57%	3.554%


Sum of corrected areas: 29686872

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
Data File : BF123213.D
Acq On : 17 Feb 2021 15:24
Operator : JU/CG
Sample : PB134684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

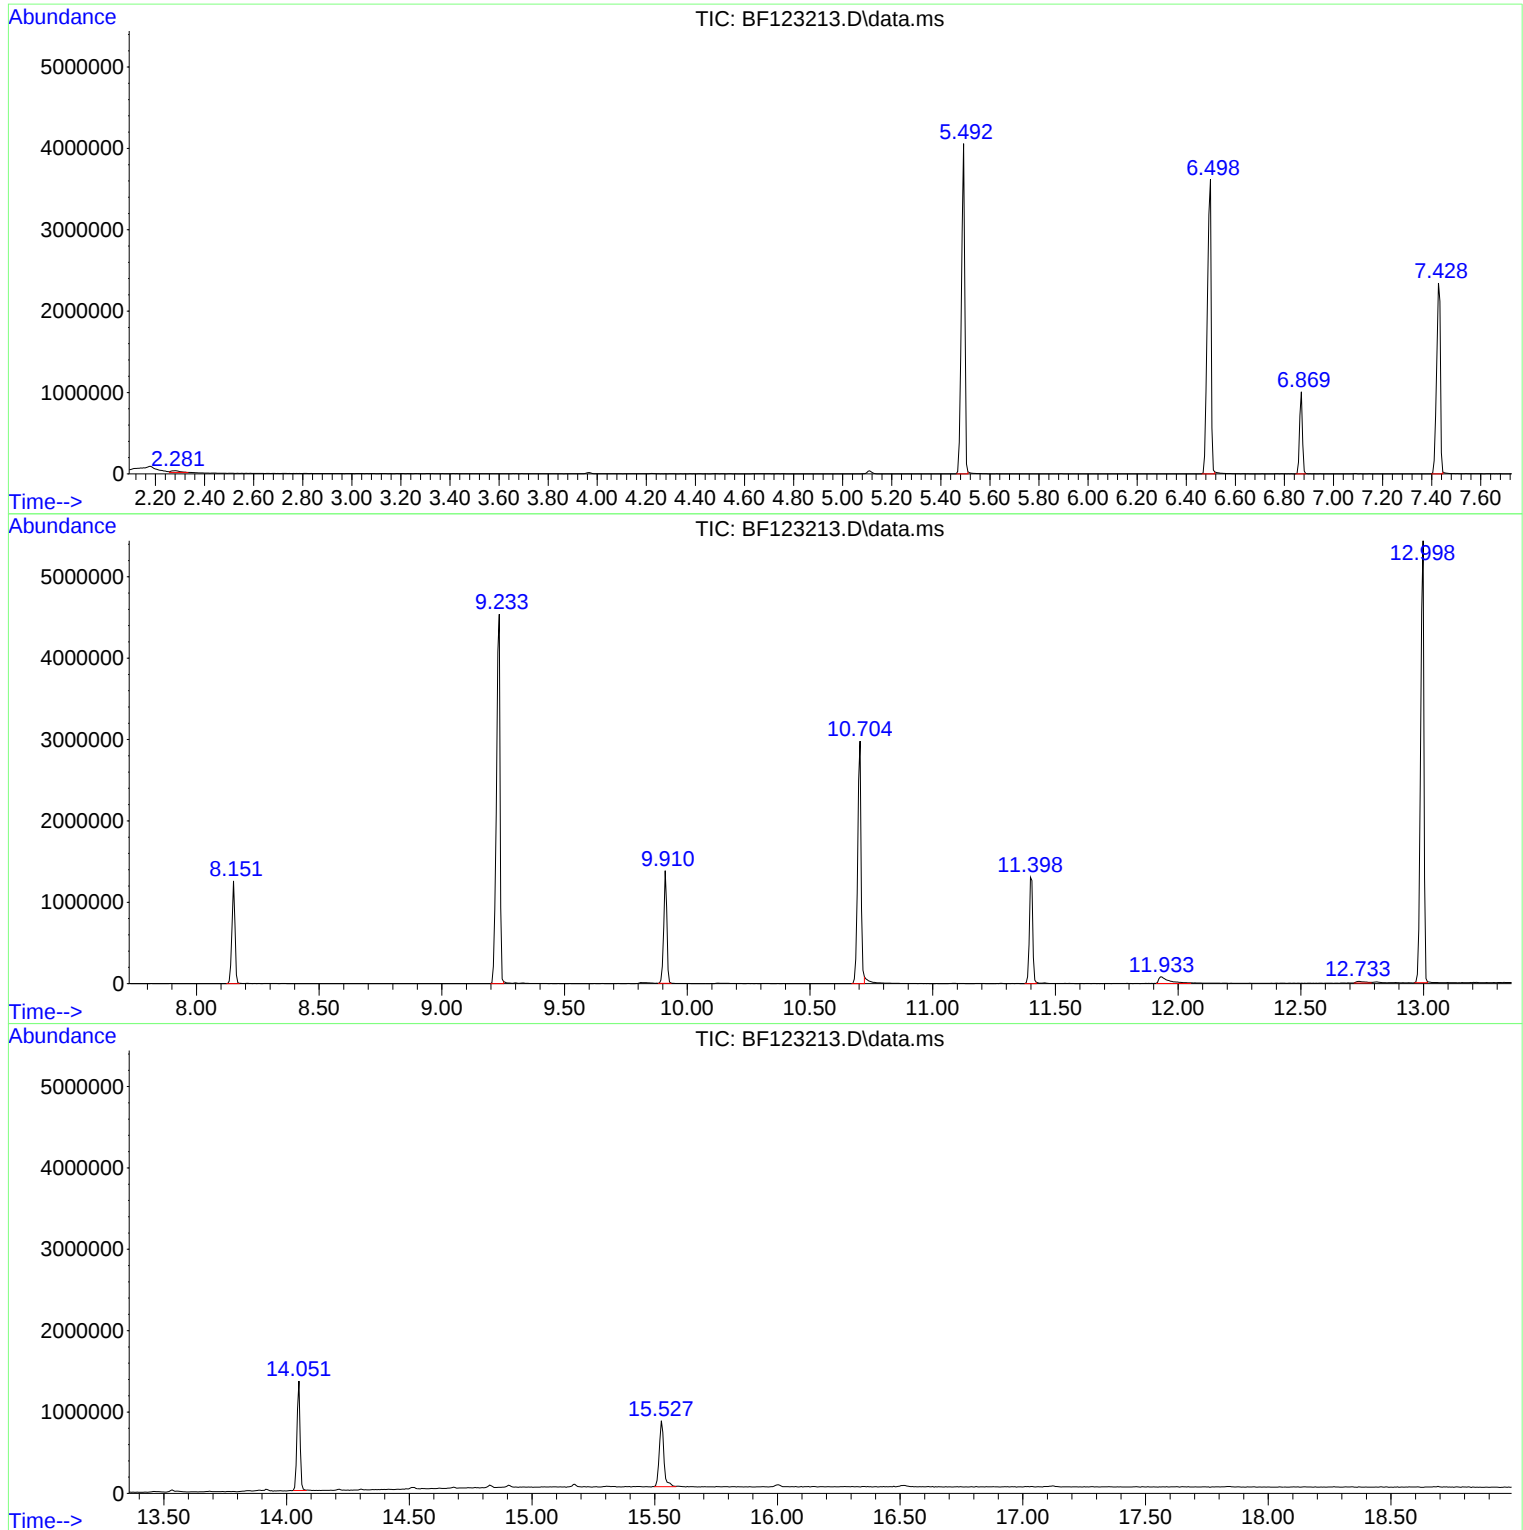

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
Data File : BF123213.D
Acq On : 17 Feb 2021 15:24
Operator : JU/CG
Sample : PB134684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
Data File : BF123213.D
Acq On : 17 Feb 2021 15:24
Operator : JU/CG
Sample : PB134684BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134684BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------