


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021721\
 Data File : BF123211.D
 Acq On : 17 Feb 2021 12:43
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 12 16:59:49 2021

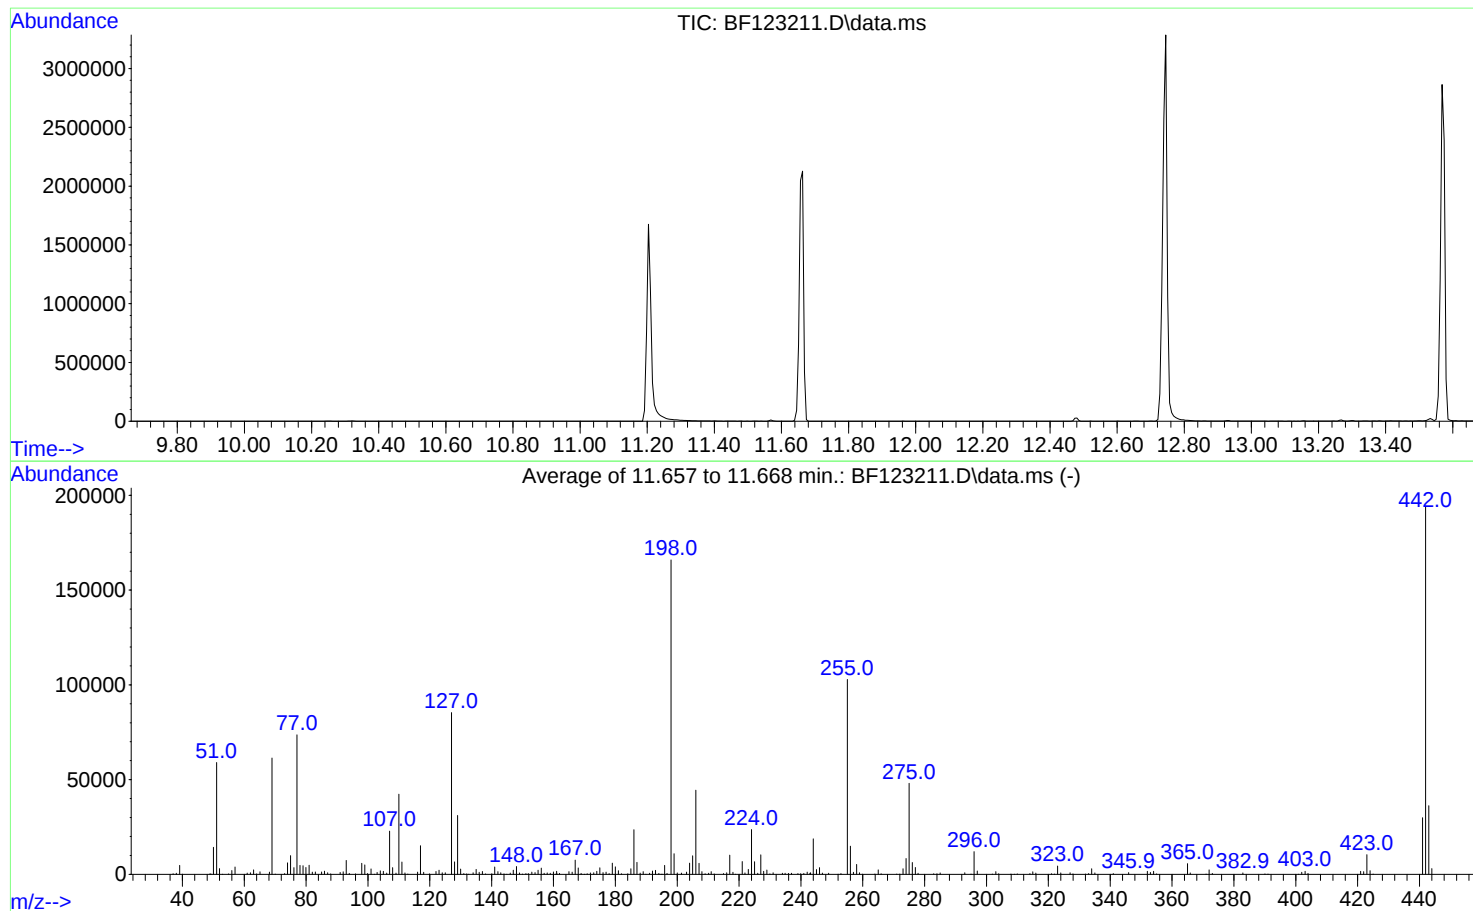




AutoFind: Scans 1627, 1628, 1629; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.6	59030	PASS
68	69	0.00	2	2.0	1203	PASS
69	198	0.00	100	37.0	61387	PASS
70	69	0.00	2	0.3	172	PASS
127	198	10	80	51.4	85330	PASS
197	198	0.00	2	0.3	534	PASS
198	198	100	100	100.0	165944	PASS
199	198	5	9	6.5	10856	PASS
275	198	10	60	28.9	48032	PASS
365	198	1	100	3.4	5653	PASS
441	198	0.01	100	18.0	29872	PASS
442	442	50	100	100.0	194117	PASS
443	442	15	24	18.7	36227	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021821\
Data File : BF123223.D
Acq On : 18 Feb 2021 11:27
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 12:41:59 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 12 16:59:49 2021
Response via : Initial Calibration

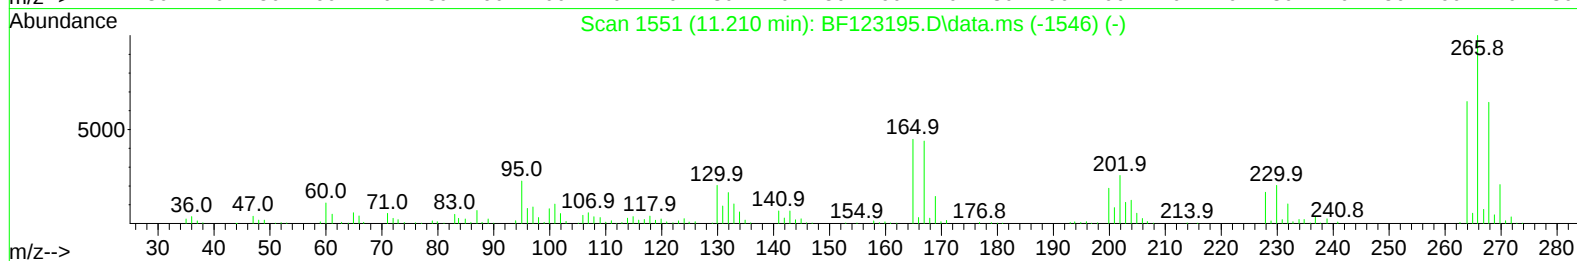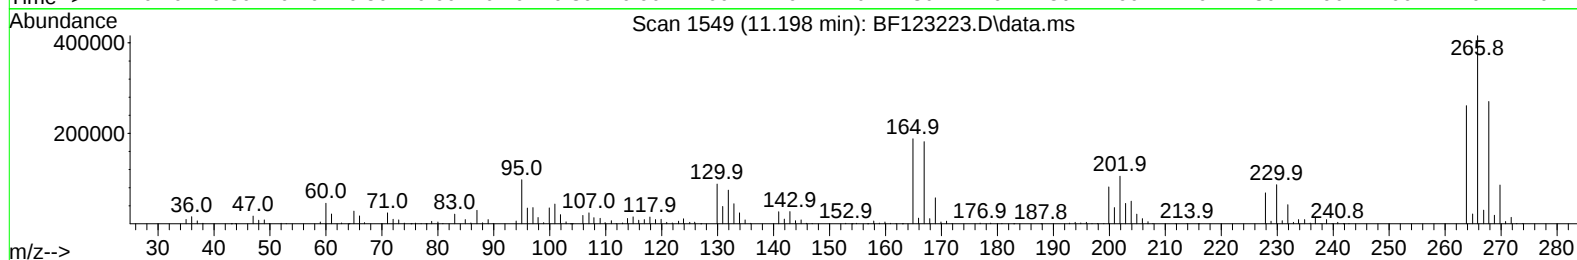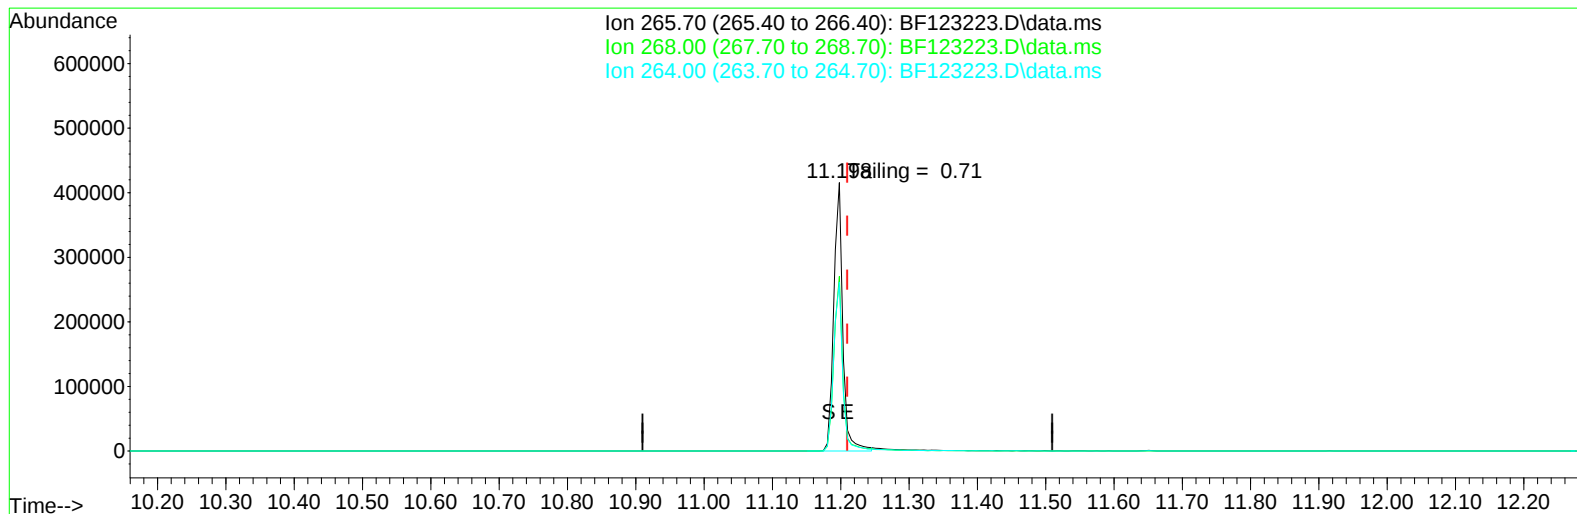

TIC: BF123223.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.012) 479122.79 ng




response 385325

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.02
264.00	62.30	62.88
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021821\
 Data File : BF123223.D
 Acq On : 18 Feb 2021 11:27
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 18 12:41:59 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 12 16:59:49 2021
 Response via : Initial Calibration

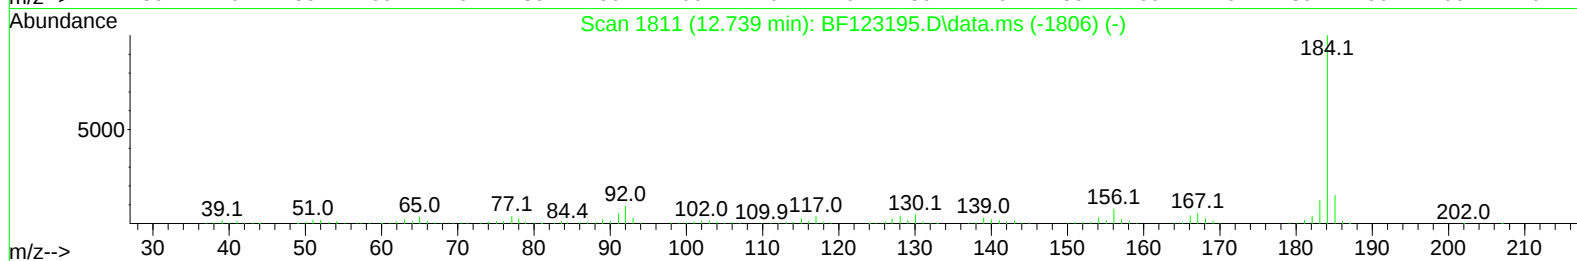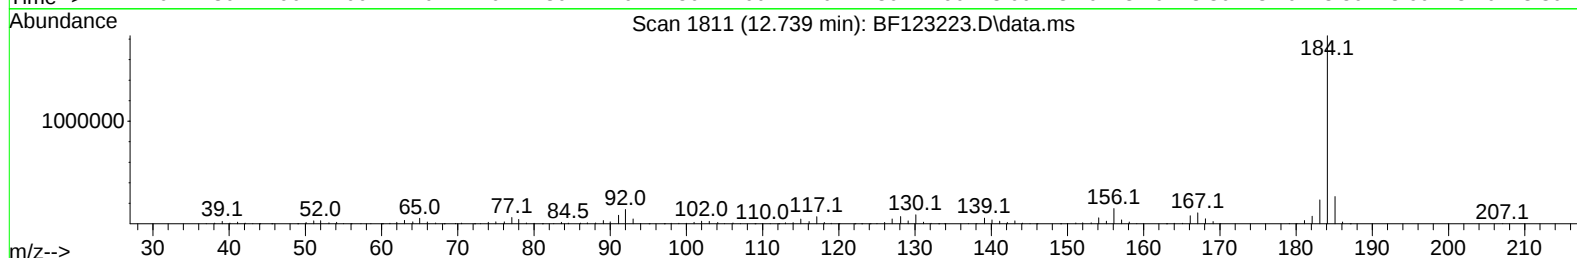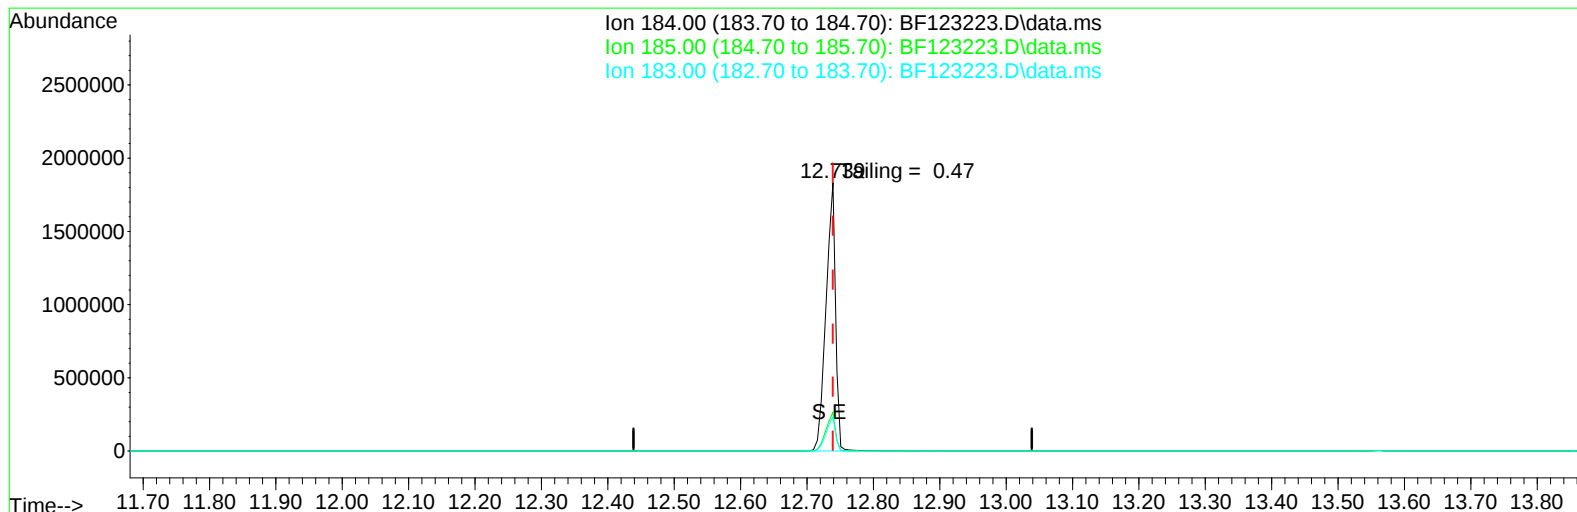

TIC: BF123223.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 76430.87 ng

response 1833250

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.51
183.00	12.10	12.72
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
02/17/2021	BNA_F	<u>BF123211.D</u>
Compound Name	Response	Retention Time
DDT	485079	13.56
DDD	2686	13.26
DDE	1175	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3861	488940	0.79

Instrument :
BNA_F
ClientSampleId :
DFTPP