
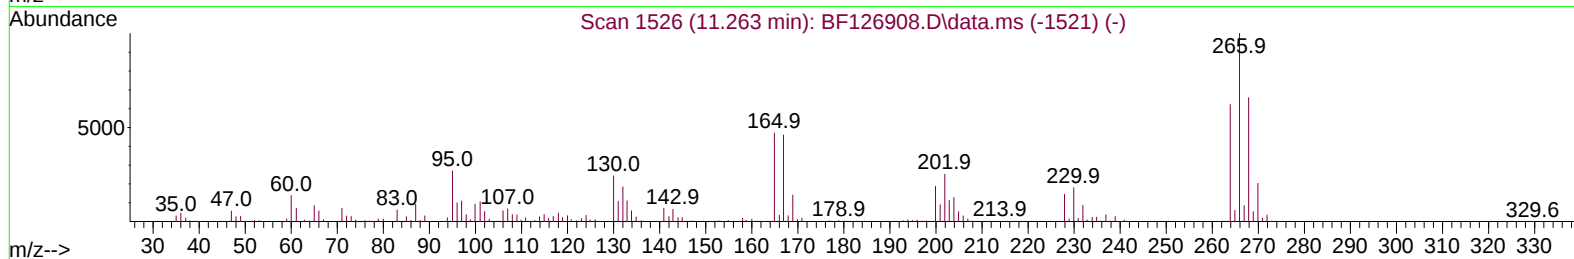
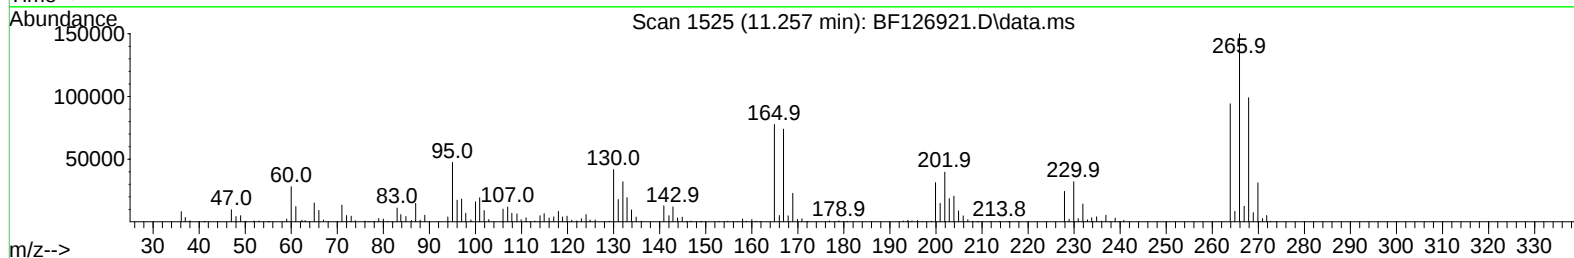


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021722\
Data File : BF126921.D
Acq On : 17 Feb 2022 10:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 17:17:14 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

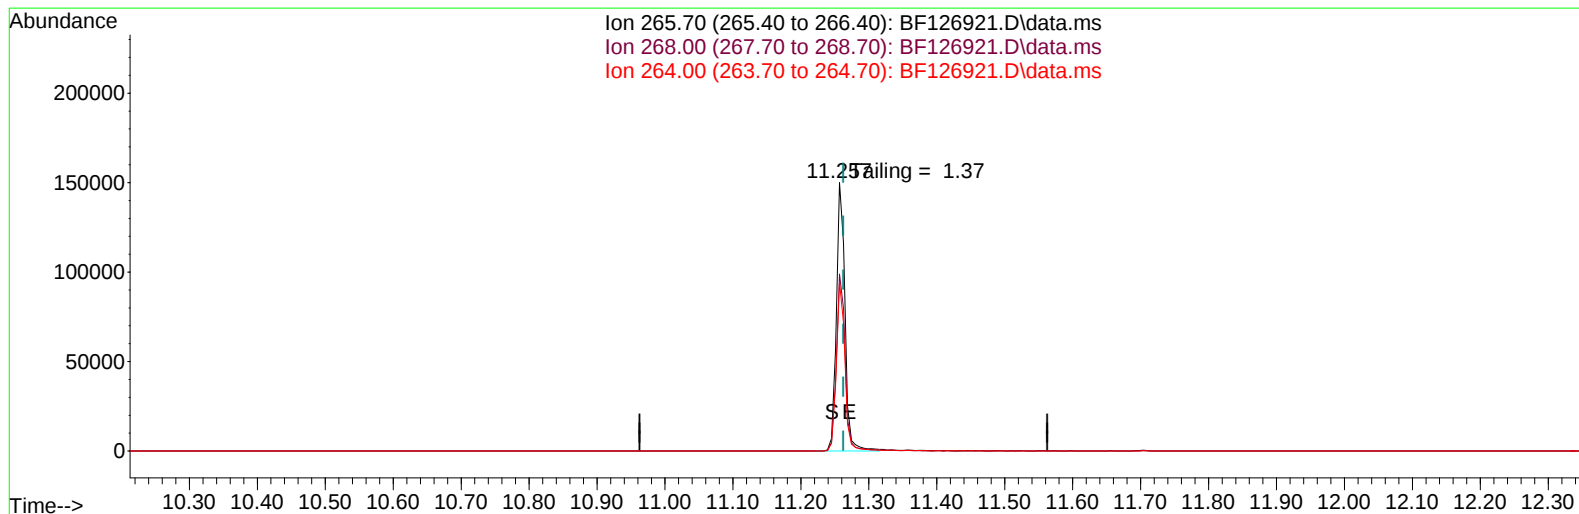

TIC: BF126921.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.006) 255492.68 ng

response 132527

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	65.97
264.00	63.00	62.78
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021722\
 Data File : BF126921.D
 Acq On : 17 Feb 2022 10:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 17 17:17:14 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 14:55:48 2022
 Response via : Initial Calibration

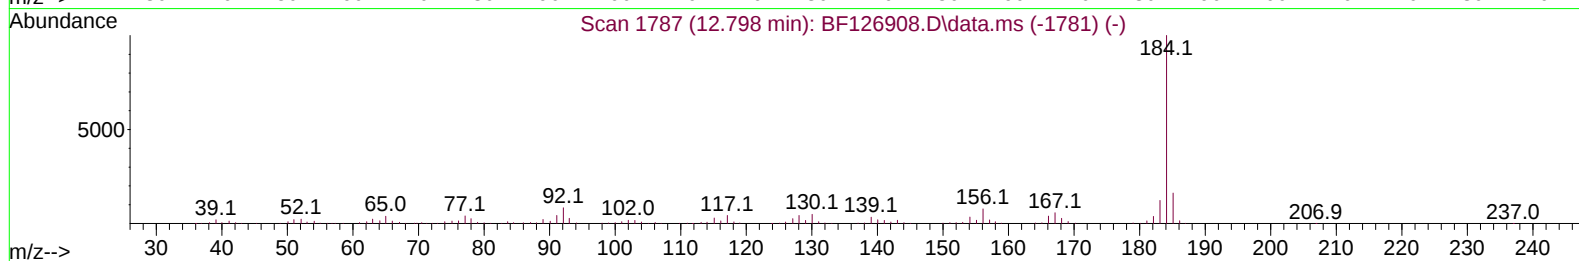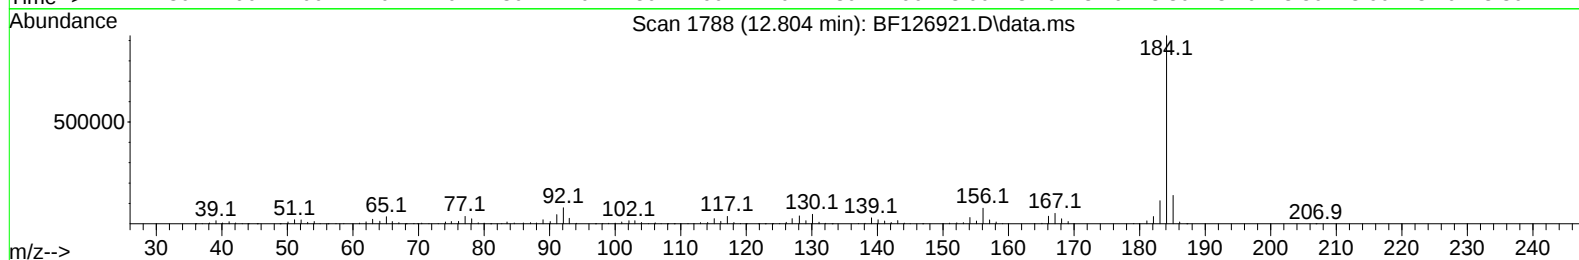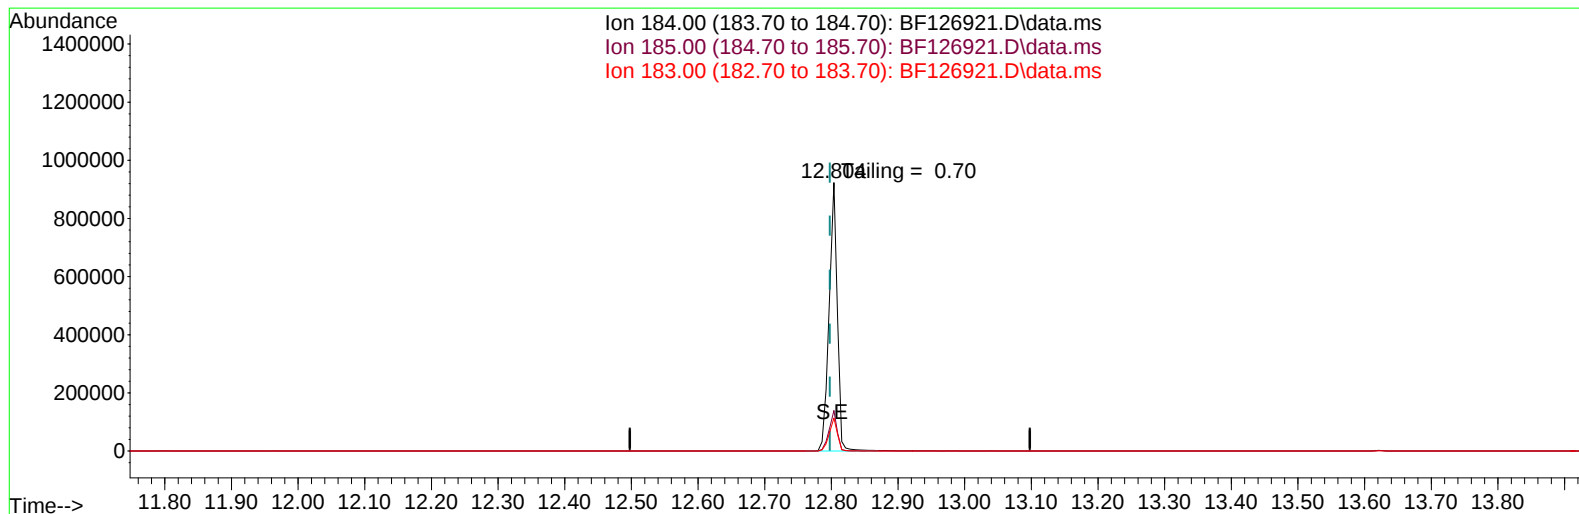

TIC: BF126921.D\data.ms

(77) Benzidine**12.804min (+ 0.006) 33644.92 ng****response 794547**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	15.10
183.00	10.20	12.27#
0.00	0.00	0.00