

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021815\
 Data File : BF077366.D
 Acq On : 18 Feb 2015 21:56
 Operator : TP/IZ
 Sample : PB81756BL
 Misc : W
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB81756BL

Quant Time: Feb 19 03:31:44 2015
 Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 18 09:51:00 2015
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.36	152	57531	20.00	ng	-0.02
21) Naphthalene-d8	8.93	136	226857	20.00	ng	-0.02
38) Acenaphthene-d10	11.10	164	111434	20.00	ng	-0.03
63) Phenanthrene-d10	12.96	188	233254	20.00	ng	-0.02
75) Chrysene-d12	16.26	240	225573	20.00	ng	-0.01
86) Perylene-d12	18.02	264	226775	20.00	ng	0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.65	112	387414	115.08	ng	-0.01
7) Phenol-d6	6.90	99	455663	103.61	ng	-0.02
23) Nitrobenzene-d5	8.04	82	269215	82.18	ng	-0.02
41) 2,4,6-Tribromophenol	12.09	330	141234	136.00	ng	-0.02
44) 2-Fluorobiphenyl	10.28	172	664915	89.95	ng	-0.02
78) Terphenyl-d14	14.96	244	756610	76.26	ng	-0.02
Target Compounds						
83) Bis(2-ethylhexyl)phthalate	16.29	149	1244	Below Cal	Qvalue #	57


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021815\
Data File : BF077366.D
Acq On : 18 Feb 2015 21:56
Operator : TP/IZ
Sample : PB81756BL
Misc : W
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB81756BL

Quant Time: Feb 19 03:31:44 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 09:51:00 2015
Response via : Initial Calibration

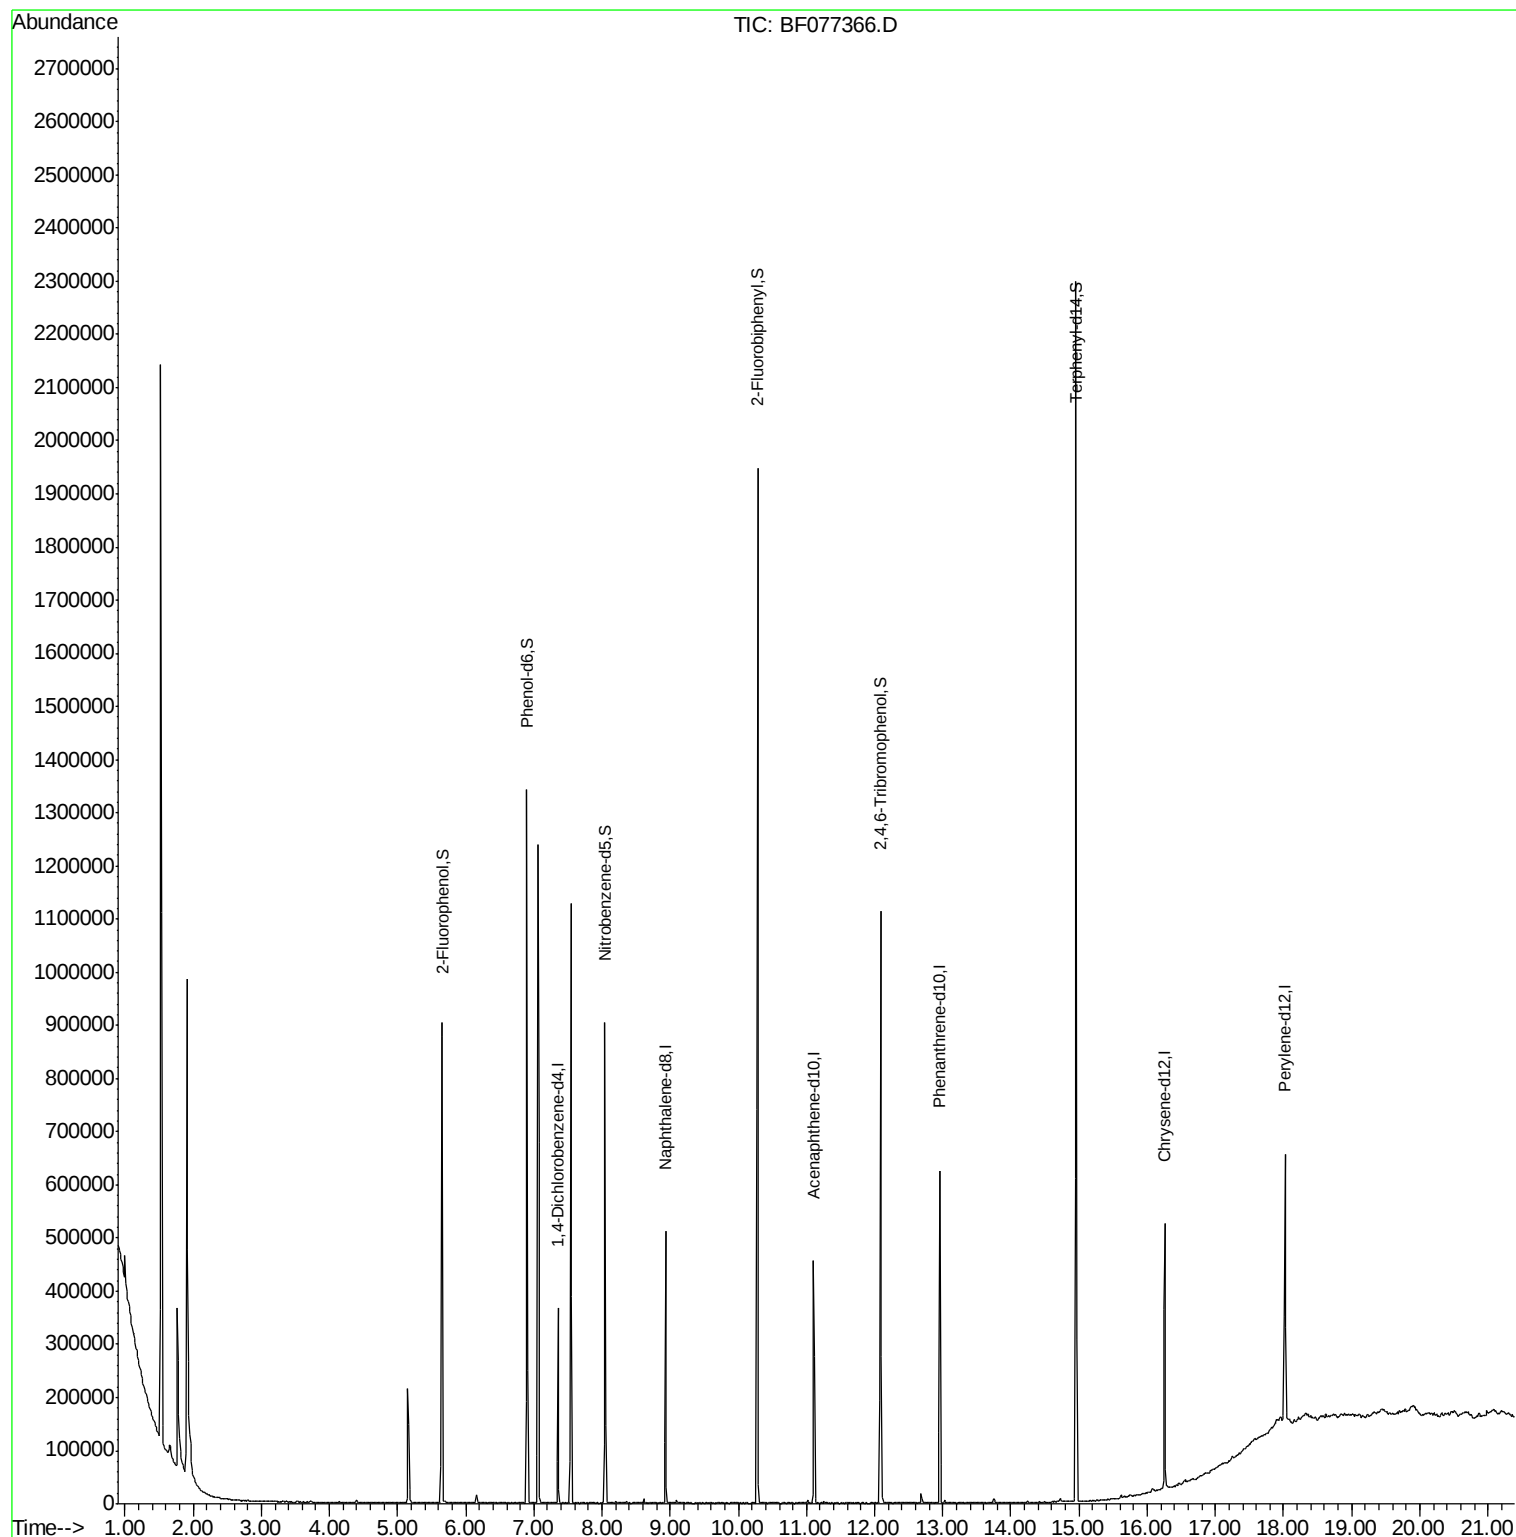


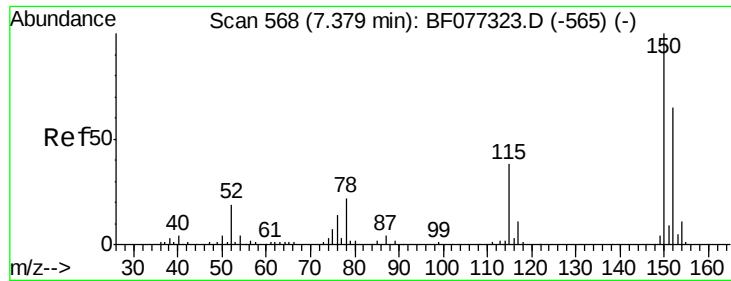




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.00 ng
 RT: 7.36 min Scan# 566
 Delta R.T. -0.02 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Instrument :
 BNA_F
 ClientSampleId :
 PB81756BL

Tgt Ion:152 Resp: 57531
 Ion Ratio Lower Upper
 152 100
 150 150.4 123.1 184.7
 115 54.1 46.2 69.4




Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

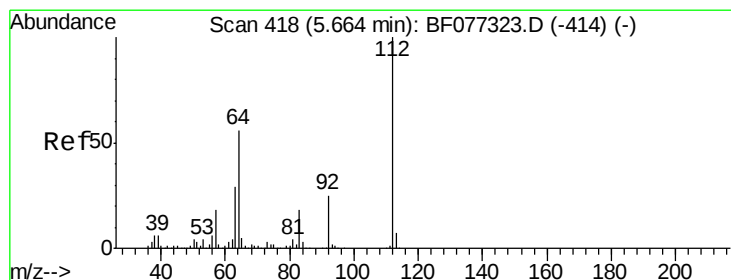
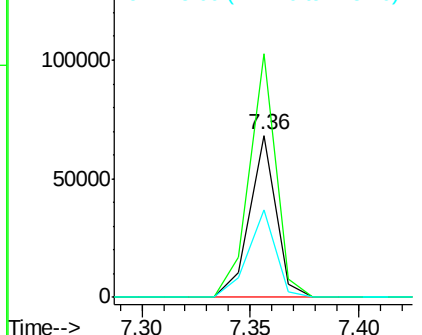



#5
 2-Fluorophenol
 Concen: 115.08 ng
 RT: 5.65 min Scan# 417
 Delta R.T. -0.01 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Tgt Ion:112 Resp: 387414
 Ion Ratio Lower Upper
 112 100
 64 47.6 44.7 67.1
 63 24.6 23.3 34.9



Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF0
 Ion 63.00 (62.70 to 63.70): BF0

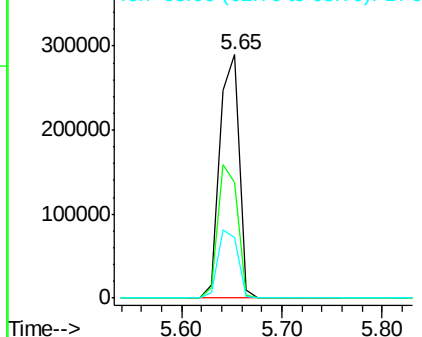

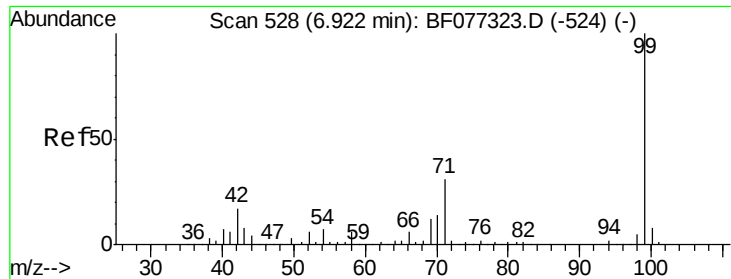

#7

Phenol-d6

Concen: 103.61 ng

RT: 6.90 min Scan# 526

Delta R.T. -0.02 min

Lab File: BF077366.D

Acq: 18 Feb 2015 21:56

Instrument :

BNA_F

ClientSampleId :

PB81756BL


Tgt Ion: 99 Resp: 455663

Ion Ratio Lower Upper

99 100

42 18.7 13.8 20.6




71 32.8 24.6 37.0

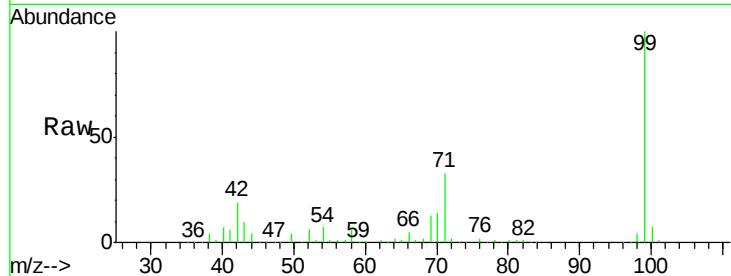

Abundance Ion 99.00 (98.70 to 99.70): BF0

Ion 42.00 (41.70 to 42.70): BF0

Ion 71.00 (70.70 to 71.70): BF0

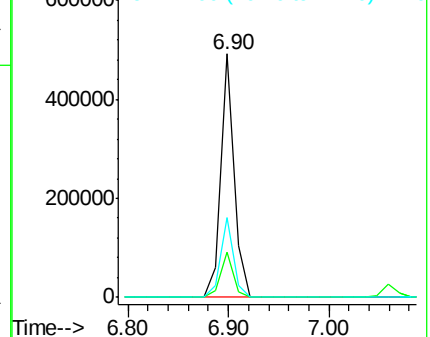

#21

Naphthalene-d8

Concen: 20.00 ng

RT: 8.93 min Scan# 704

Delta R.T. -0.02 min

Lab File: BF077366.D

Acq: 18 Feb 2015 21:56

Tgt Ion: 136 Resp: 226857


Ion Ratio Lower Upper

136 100

137 11.4 8.7 13.1

54 6.8 5.8 8.6

68 5.6 4.6 6.8






Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF0

Ion 68.00 (67.70 to 68.70): BF0

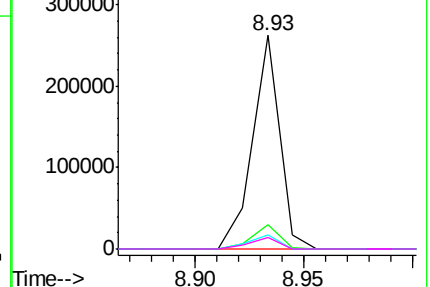







#23
 Nitrobenzene-d5
 Concen: 82.18 ng
 RT: 8.04 min Scan# 626
 Delta R.T. -0.02 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Instrument :
 BNA_F
 ClientSampleId :
 PB81756BL

Tgt Ion	Ratio	Lower	Upper
82	100		
128	43.5	30.7	46.1
54	50.5	43.1	64.7

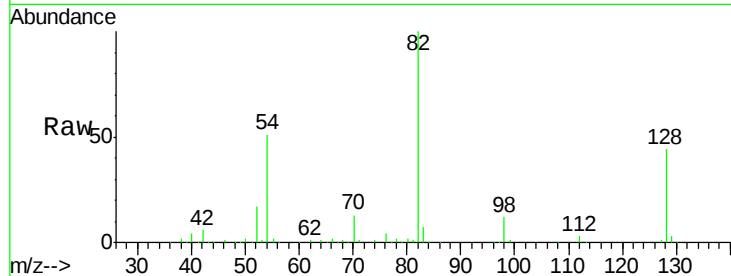


Abundance Ion 82.00 (81.70 to 82.70): BF0
 Ion 128.00 (127.70 to 128.70): B
 Ion 54.00 (53.70 to 54.70): BF0

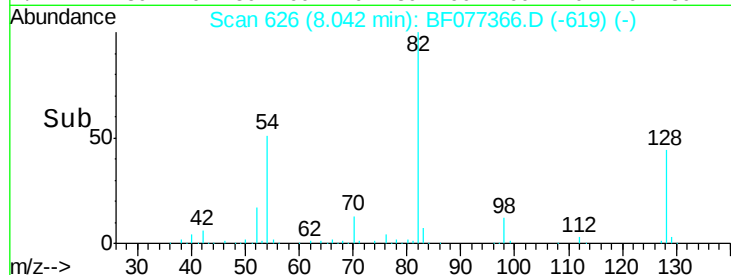
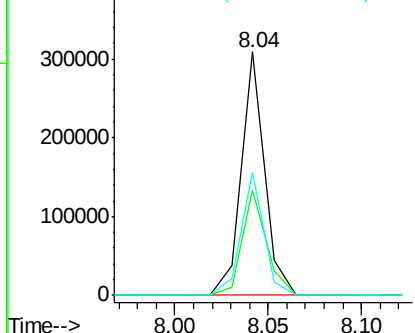



#38
 Acenaphthene-d10
 Concen: 20.00 ng
 RT: 11.10 min Scan# 894
 Delta R.T. -0.03 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Tgt Ion	Ratio	Lower	Upper
164	100		
162	104.2	80.4	120.6
160	46.8	35.3	52.9



Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

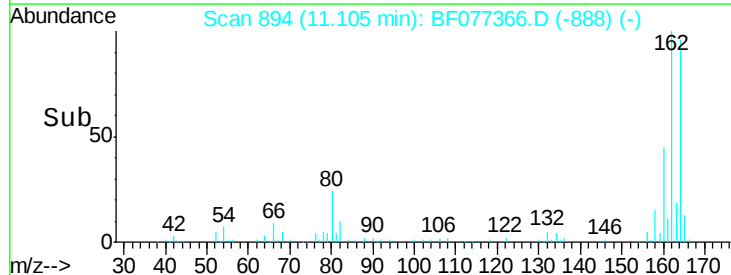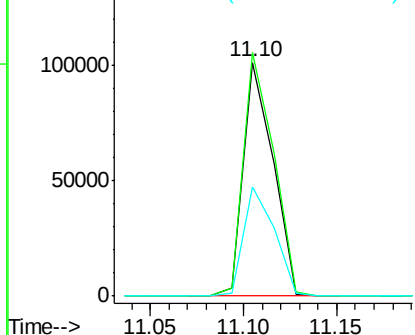







#41
 2,4,6-Tribromophenol
 Concen: 136.00 ng
 RT: 12.09 min Scan# 980
 Delta R.T. -0.02 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Instrument :
 BNA_F
 ClientSampleId :
 PB81756BL

Tgt Ion:330 Resp: 141234
 Ion Ratio Lower Upper
 330 100
 332 103.4 76.1 114.1
 141 33.4 28.5 42.7

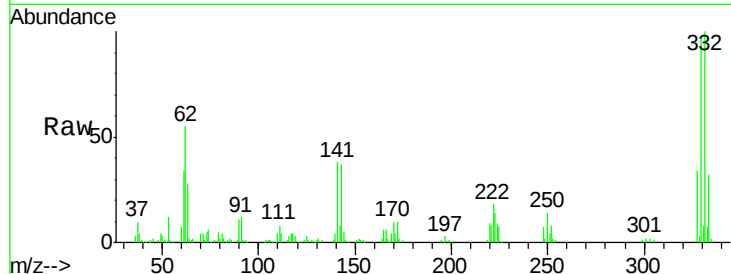


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E


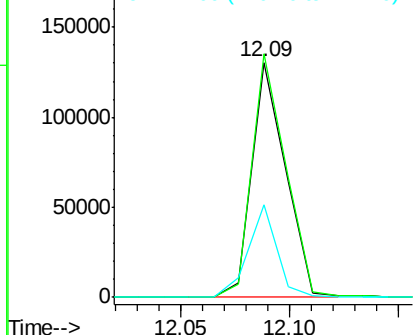



#44
 2-Fluorobiphenyl
 Concen: 89.95 ng
 RT: 10.28 min Scan# 822
 Delta R.T. -0.02 min
 Lab File: BF077366.D
 Acq: 18 Feb 2015 21:56

Tgt Ion:172 Resp: 664915
 Ion Ratio Lower Upper
 172 100
 171 35.2 28.9 43.3
 170 23.5 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

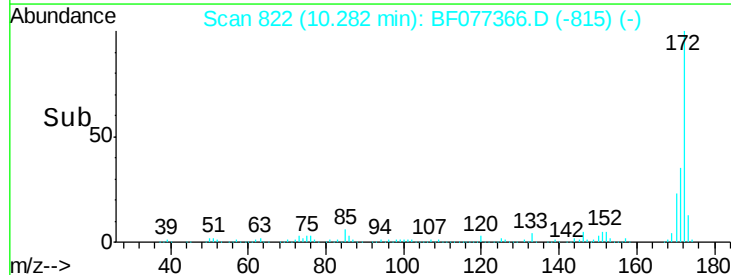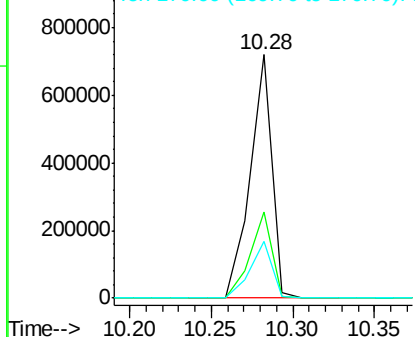


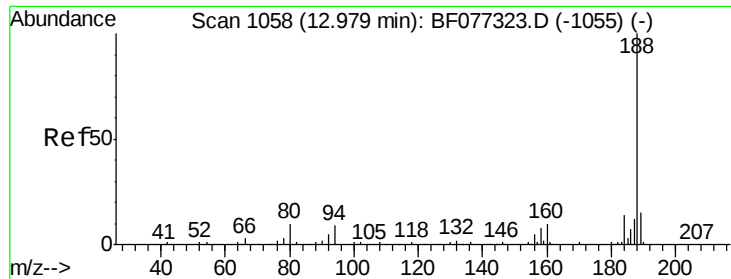




#63
Phenanthrene-d10
Concen: 20.00 ng
RT: 12.96 min Scan# 1056
Delta R.T. -0.02 min
Lab File: BF077366.D
Acq: 18 Feb 2015 21:56

Instrument :
BNA_F
ClientSampleId :
PB81756BL

Tgt Ion:188 Resp: 233254
Ion Ratio Lower Upper
188 100
94 9.4 7.2 10.8
80 9.7 7.8 11.8




Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF0
Ion 80.00 (79.70 to 80.70): BF0

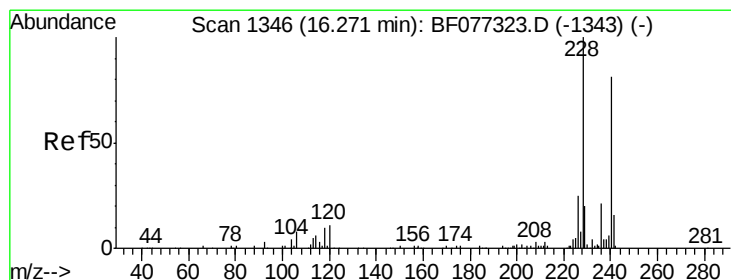
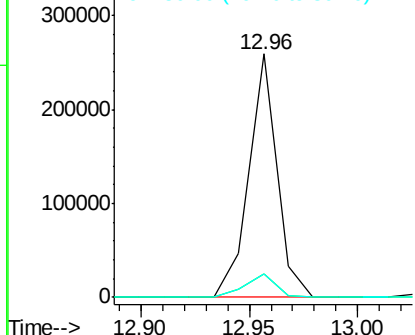



#75
Chrysene-d12
Concen: 20.00 ng
RT: 16.26 min Scan# 1345
Delta R.T. -0.01 min
Lab File: BF077366.D
Acq: 18 Feb 2015 21:56

Tgt Ion:240 Resp: 225573
Ion Ratio Lower Upper
240 100
120 9.8 11.3 16.9#
236 25.5 20.3 30.5

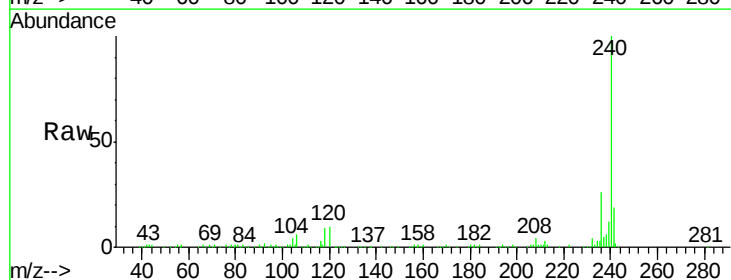

Abundance Ion 240.00 (239.70 to 240.70): E
Ion 120.00 (119.70 to 120.70): E
Ion 236.00 (235.70 to 236.70): E

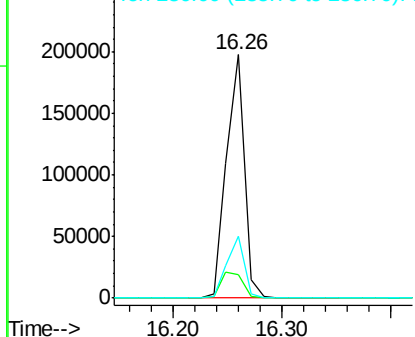

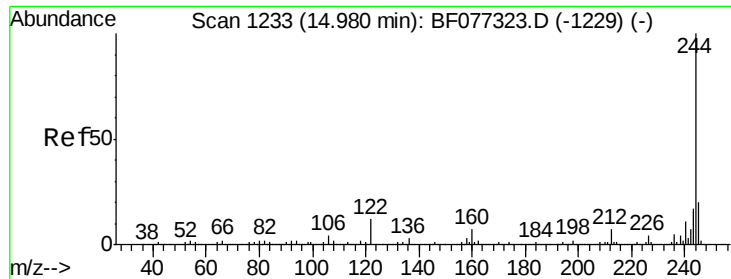

#78

Terphenyl-d14

Concen: 76.26 ng

RT: 14.96 min Scan# 1231

Delta R.T. -0.02 min

Lab File: BF077366.D

Acq: 18 Feb 2015 21:56

Instrument :

BNA_F

ClientSampleId :

PB81756BL


Tgt Ion:244 Resp: 756610

Ion Ratio Lower Upper

244 100

212 7.1 5.4 8.0




122 12.8 9.3 13.9



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

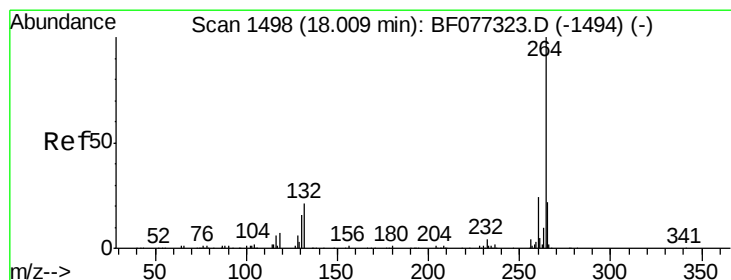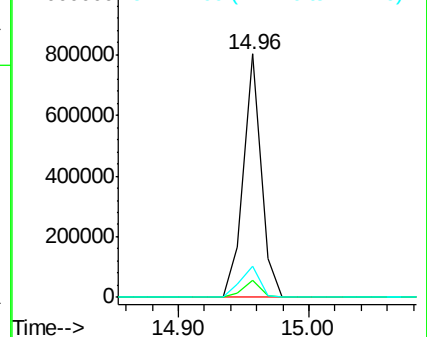

#86

Perylene-d12

Concen: 20.00 ng

RT: 18.02 min Scan# 1499

Delta R.T. 0.01 min

Lab File: BF077366.D

Acq: 18 Feb 2015 21:56


Tgt Ion:264 Resp: 226775

Ion Ratio Lower Upper

264 100

260 23.4 18.9 28.3

265 22.1 17.7 26.5

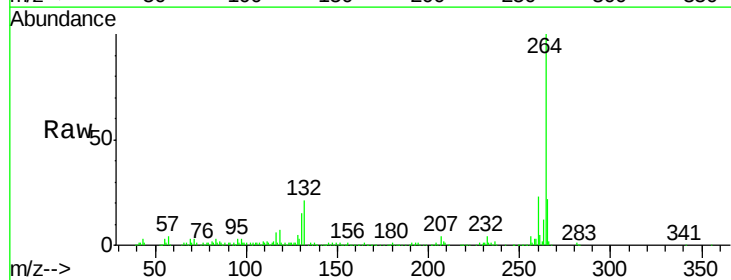

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

