


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM021815\
 Data File : BM000541.D
 Acq On : 18 Feb 2015 16:33
 Operator : TP/IZ
 Sample : DFTPP25
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM021815.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 01:10:38 2015

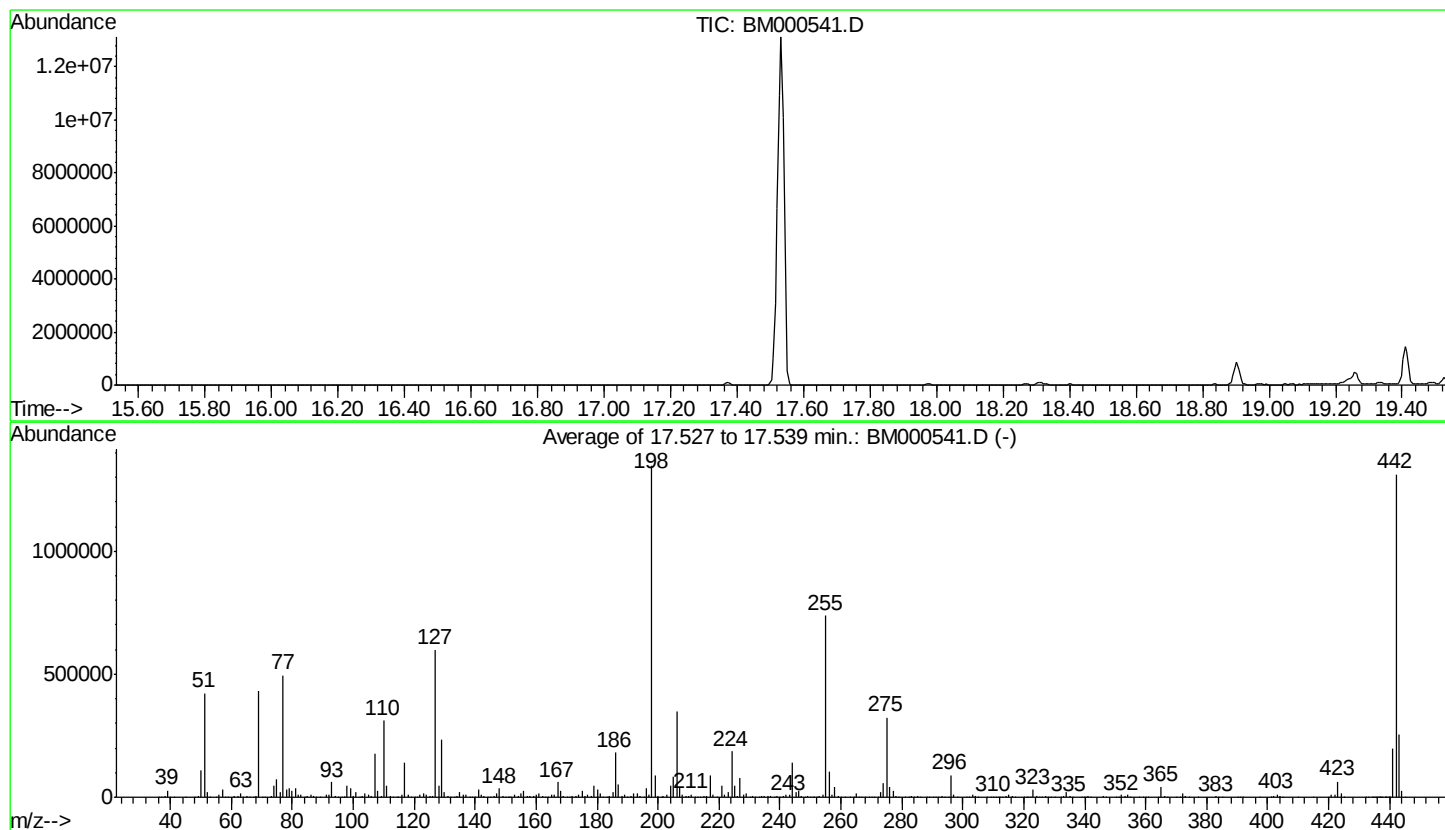

AutoFind: Scans 2523, 2524, 2525; Background Corrected with Scan 2515

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	423808	PASS
68	69	0.00	2	1.7	7202	PASS
69	198	0.00	100	31.9	430016	PASS
70	69	0.00	2	0.6	2530	PASS
127	198	10	80	44.4	598570	PASS
197	198	0.00	2	0.8	11047	PASS
198	198	100	100	100.0	1347584	PASS
199	198	5	9	6.6	89280	PASS
275	198	10	60	24.1	325120	PASS
365	198	1	100	3.2	42773	PASS
441	443	0.01	100	78.1	198058	PASS
442	198	50	100	97.4	1313066	PASS
443	442	15	24	19.3	253482	PASS