
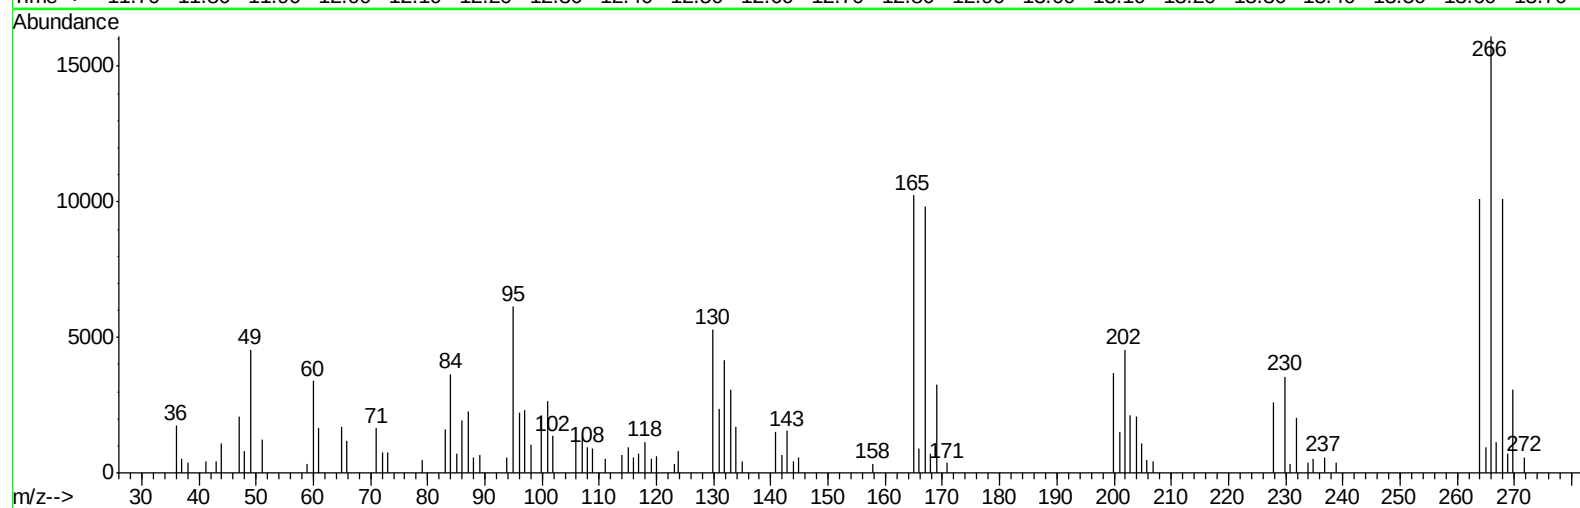


Data Path : Z:\HPCHEM1\BNA_F\Data\BF021815\
Data File : BF077353.D
Acq On : 18 Feb 2015 15:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 06:02:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 09:51:00 2015
Response via : Initial Calibration

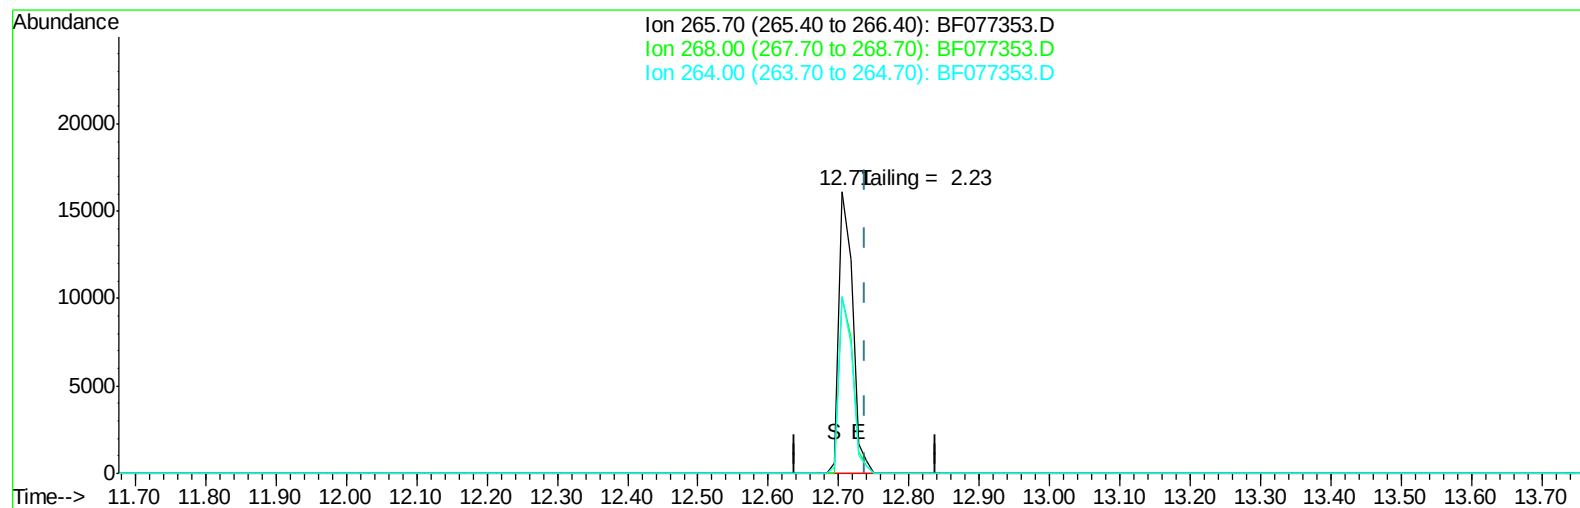

TIC: BF077353.D

(69) Pentachlorophenol (C)



12.705min (-0.034) 0.00ng

response 21474

Ion	Exp%	Act%
265.70	100	100
268.00	67.50	62.84
264.00	60.20	62.67
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_F\Data\BF021815\
Data File : BF077353.D
Acq On : 18 Feb 2015 15:32
Operator : TP/IZ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 06:02:47 2015
Quant Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021715.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 18 09:51:00 2015
Response via : Initial Calibration

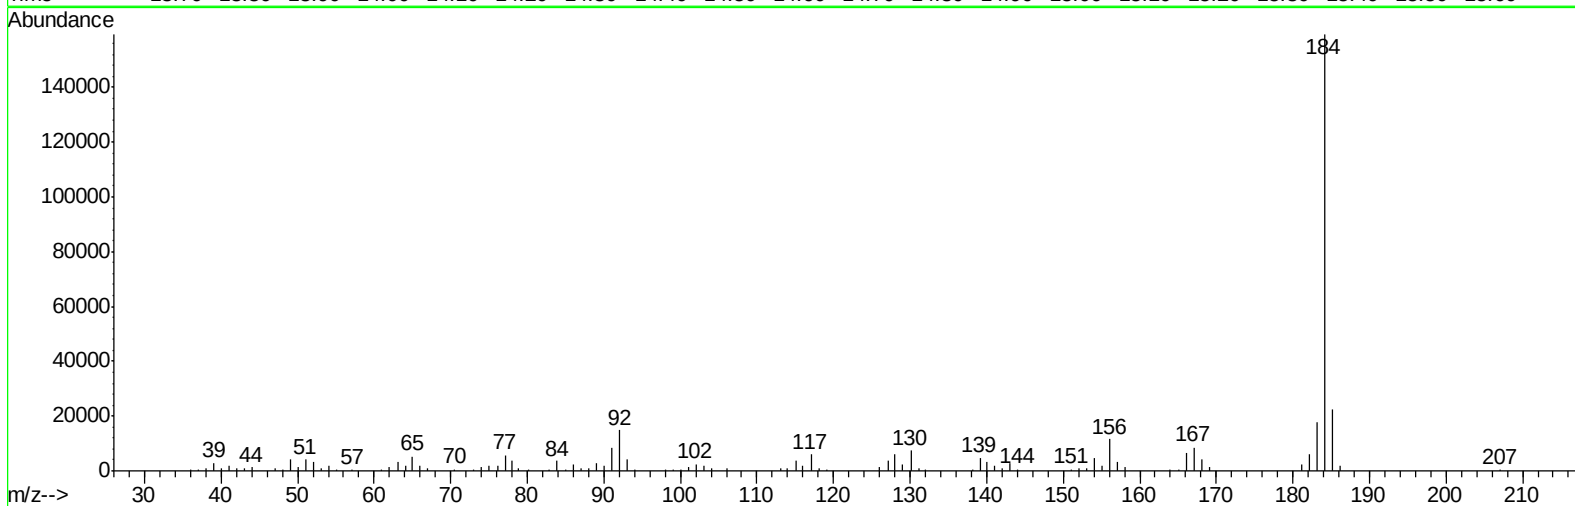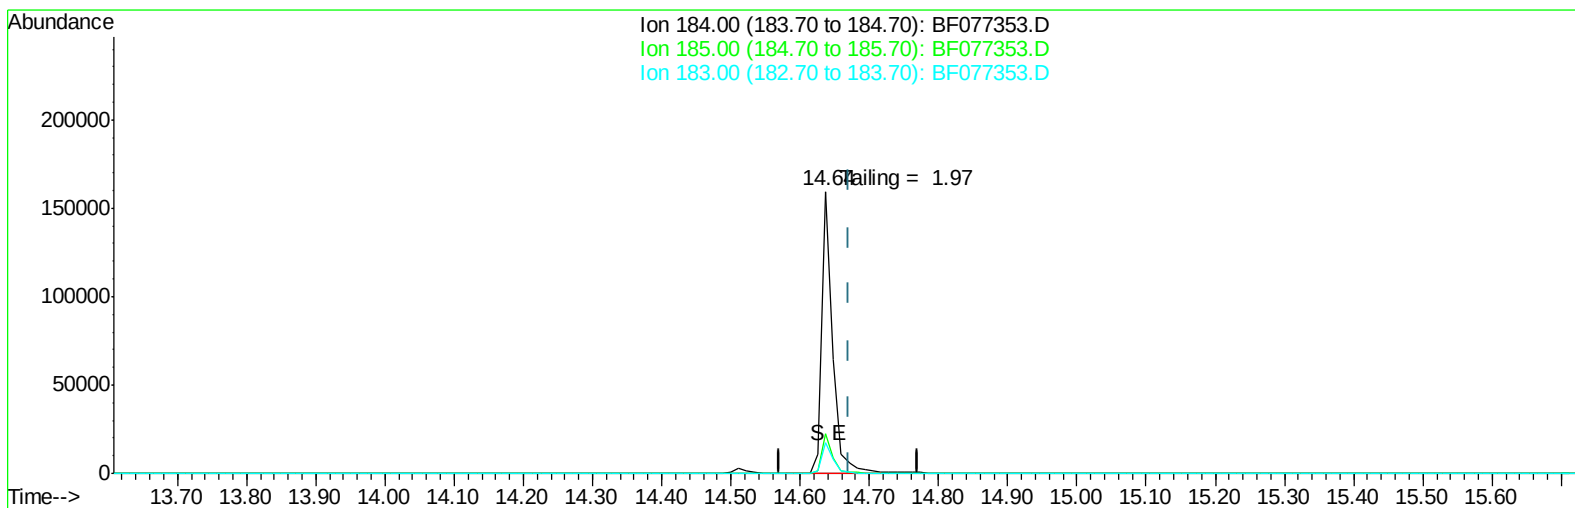

TIC: BF077353.D

(76) Benzidine

14.637min (-0.034) 0.00ng

response 177944

Ion	Exp%	Act%
184.00	100	100
185.00	15.40	14.18
183.00	11.60	11.08
0.00	0.00	0.00