
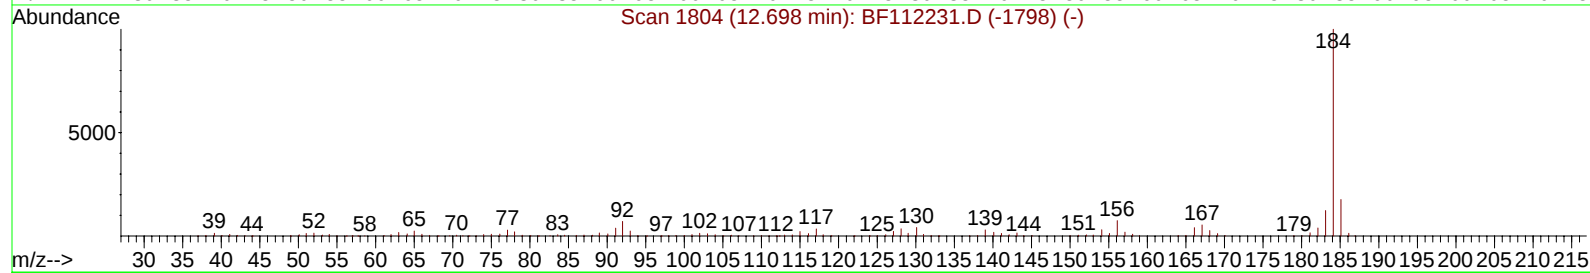
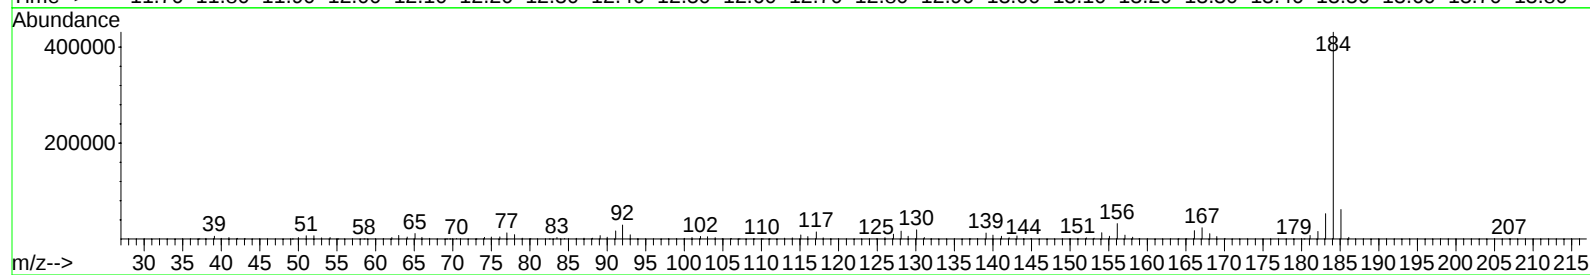


```
Data Path   : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021819\  
Data File   : BF112595.D  
Acq On      : 18 Feb 2019   12:33  
Operator    : JU/SJ  
Sample      : DFTPP  
Misc        :  
ALS Vial    : 1      Sample Multiplier: 1
```

Quant Time: Feb 18 17:18:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

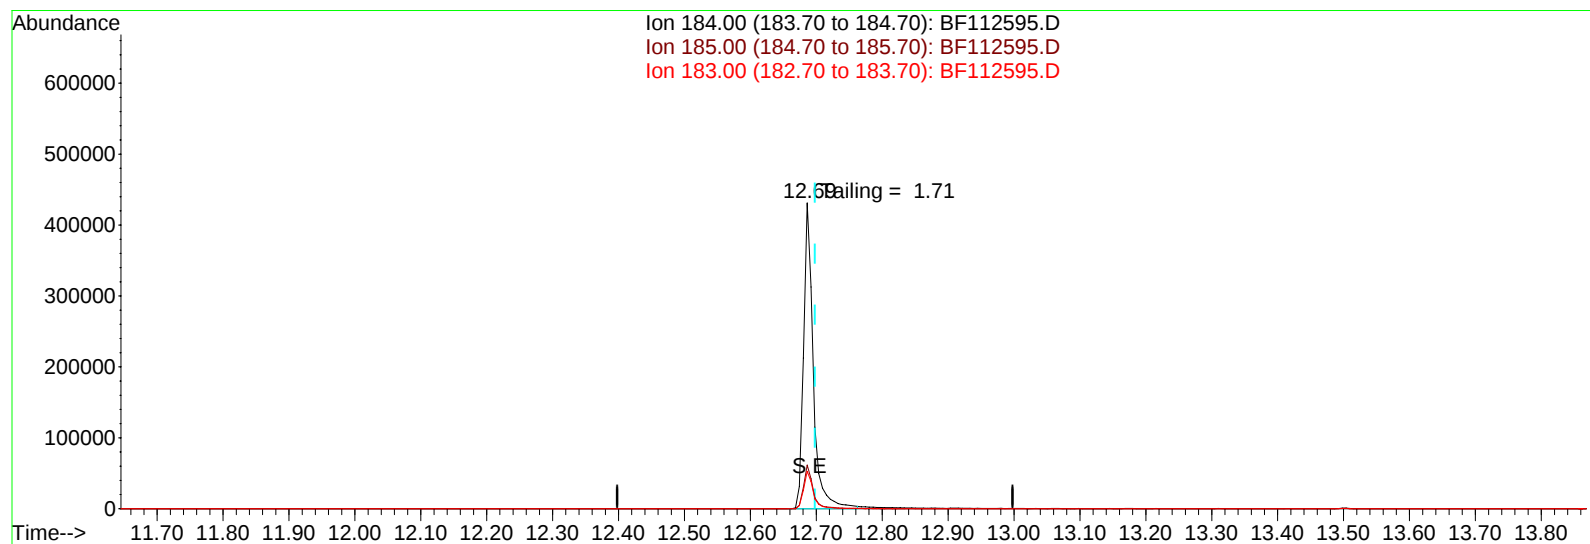

TIC: BF112595.D

(77) Benzidine




12.686min (-0.012) 0.00ng

response 453140

Ion	Exp%	Act%
184.00	100	100
185.00	17.40	14.29
183.00	12.50	12.28
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF021819\
Data File : BF112595.D
Acq On : 18 Feb 2019 12:33
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 17:18:13 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF012519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jan 28 10:38:18 2019
Response via : Initial Calibration

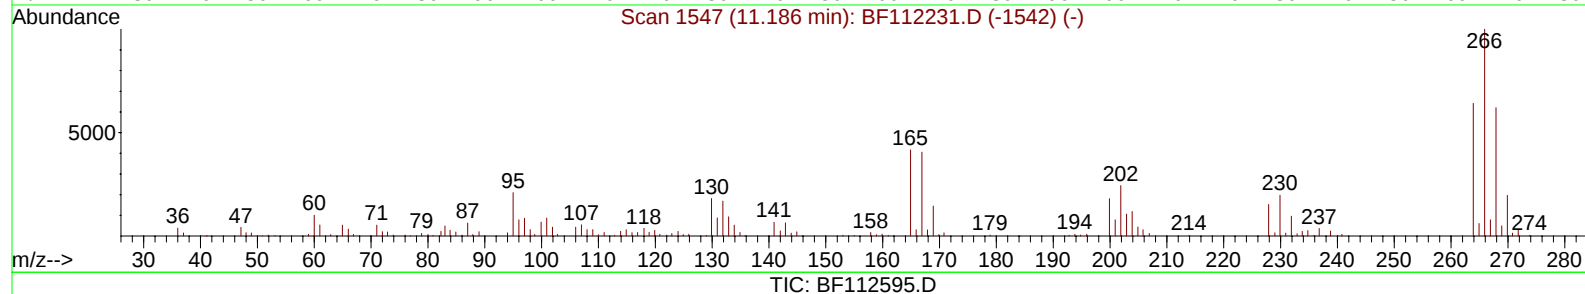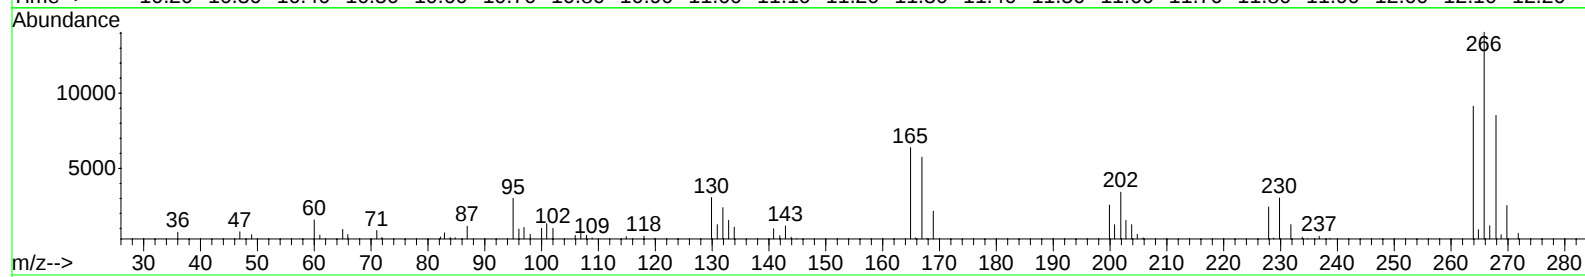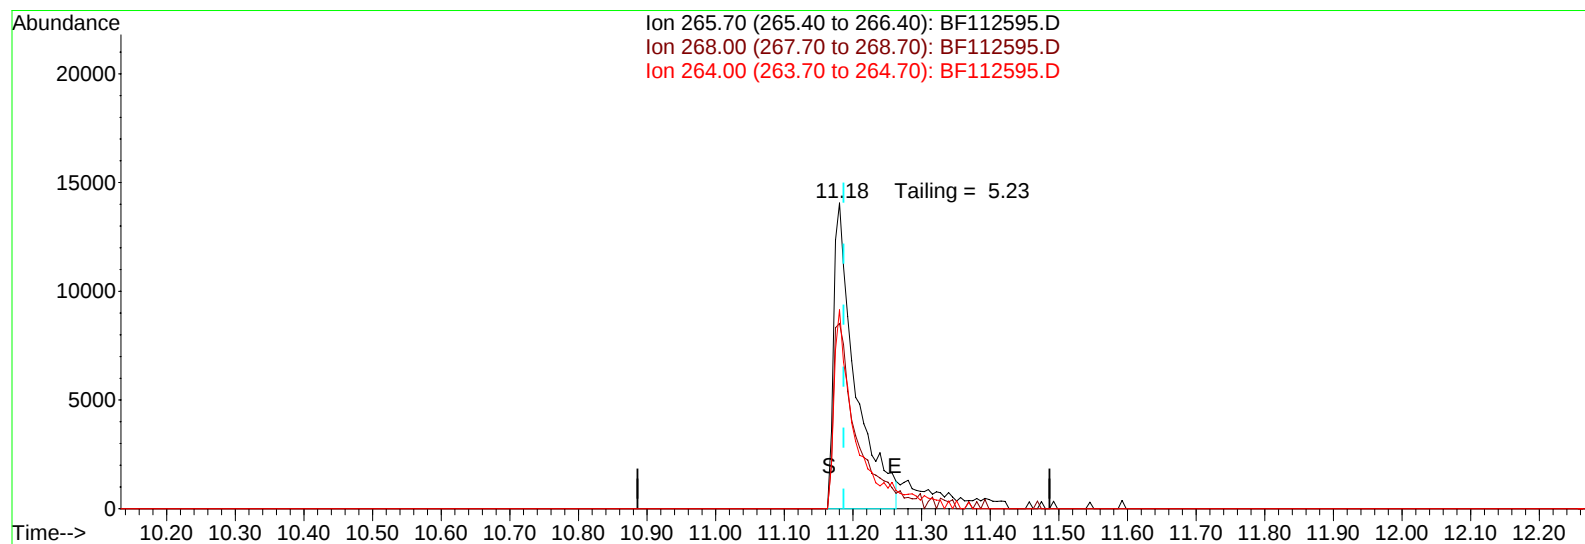

(70) Pentachlorophenol (C)

11.180min (-0.006) 21038.88ng

response 31300

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	60.64
264.00	63.60	65.03
0.00	0.00	0.00