


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF021819\
 Data File : BF112595.D
 Acq On : 18 Feb 2019 12:33
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF012519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jan 28 10:38:18 2019

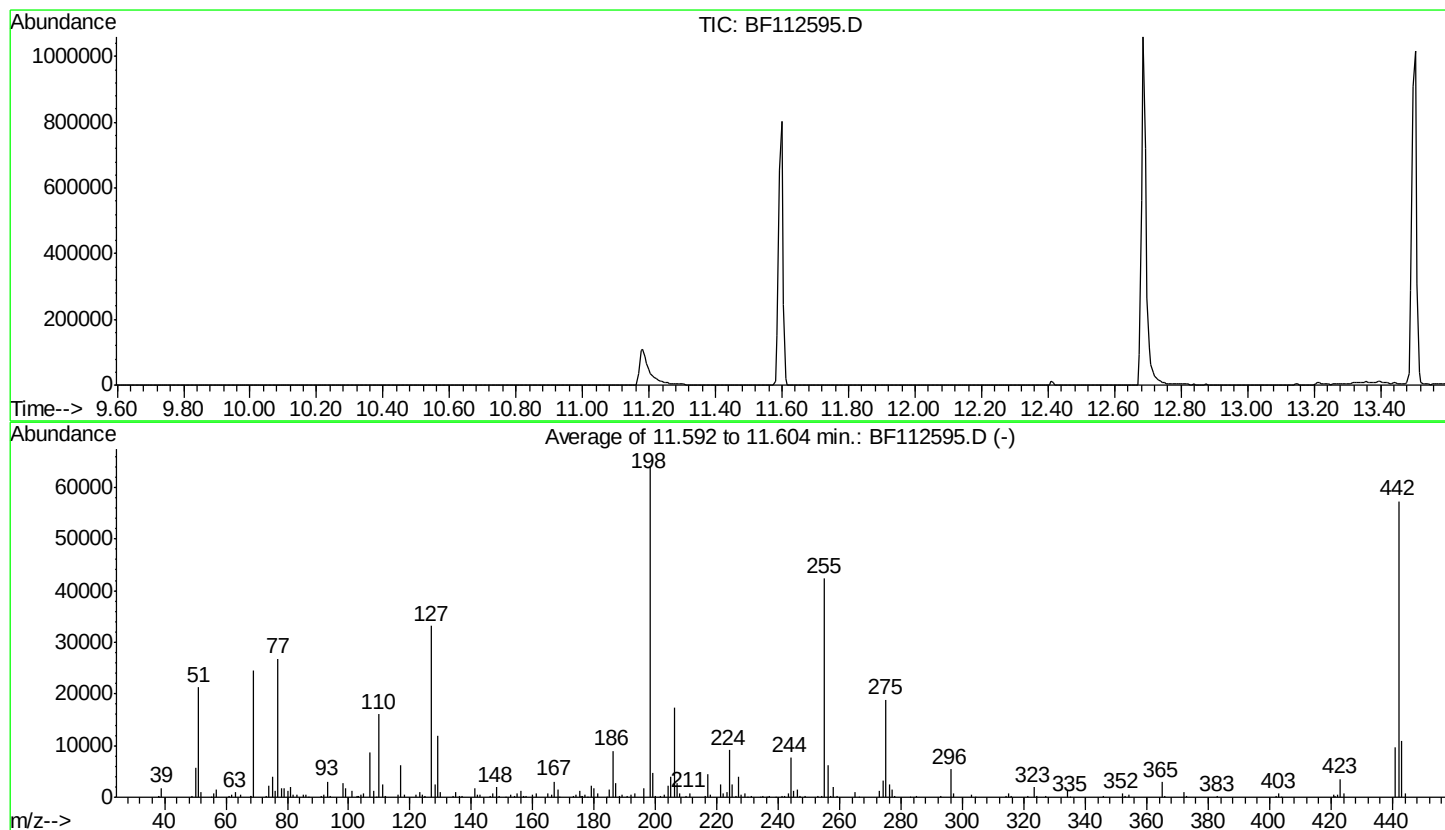

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.2	21287	PASS
68	69	0.00	2	0.9	212	PASS
69	198	0.00	100	38.1	24482	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.7	33173	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	64197	PASS
199	198	5	9	7.2	4641	PASS
275	198	10	60	29.4	18872	PASS
365	198	1	100	4.5	2896	PASS
441	198	0.01	100	15.3	9797	PASS
442	198	50	100	89.2	57269	PASS
443	442	15	24	19.2	10971	PASS