
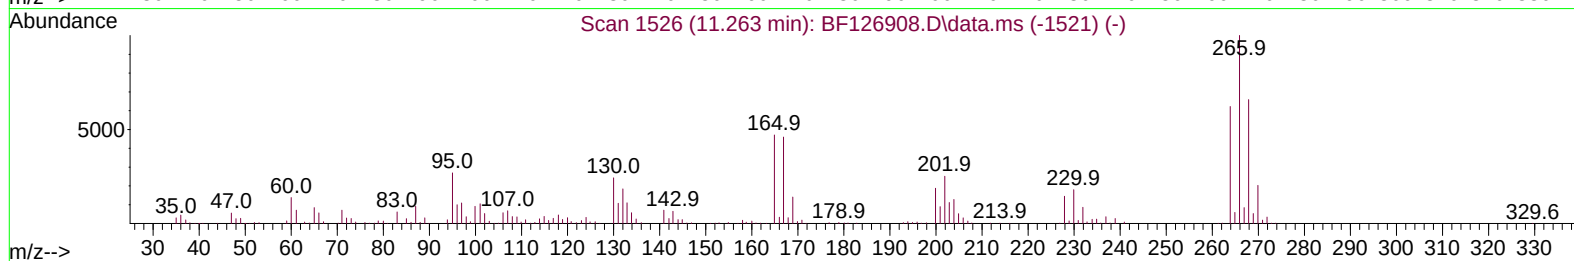
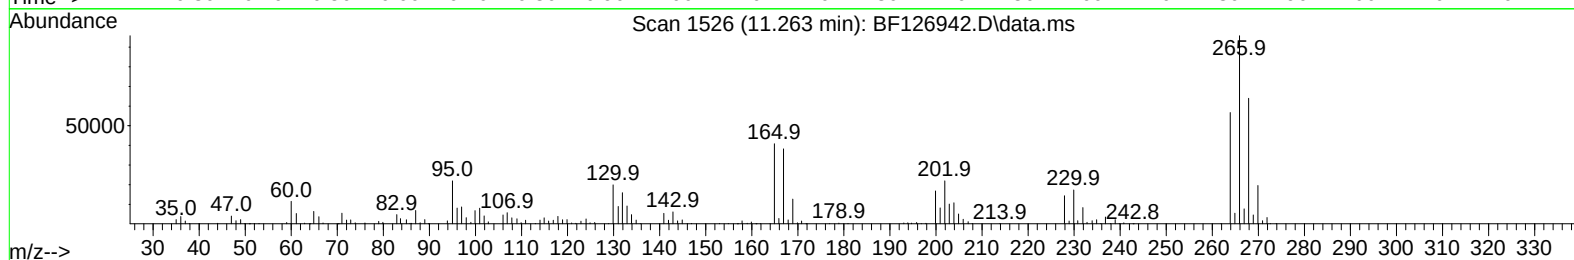


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF021822\  
 Data File : BF126942.D  
 Acq On : 18 Feb 2022 09:52  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 16:06:38 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF021622.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Feb 16 14:55:48 2022  
 Response via : Initial Calibration

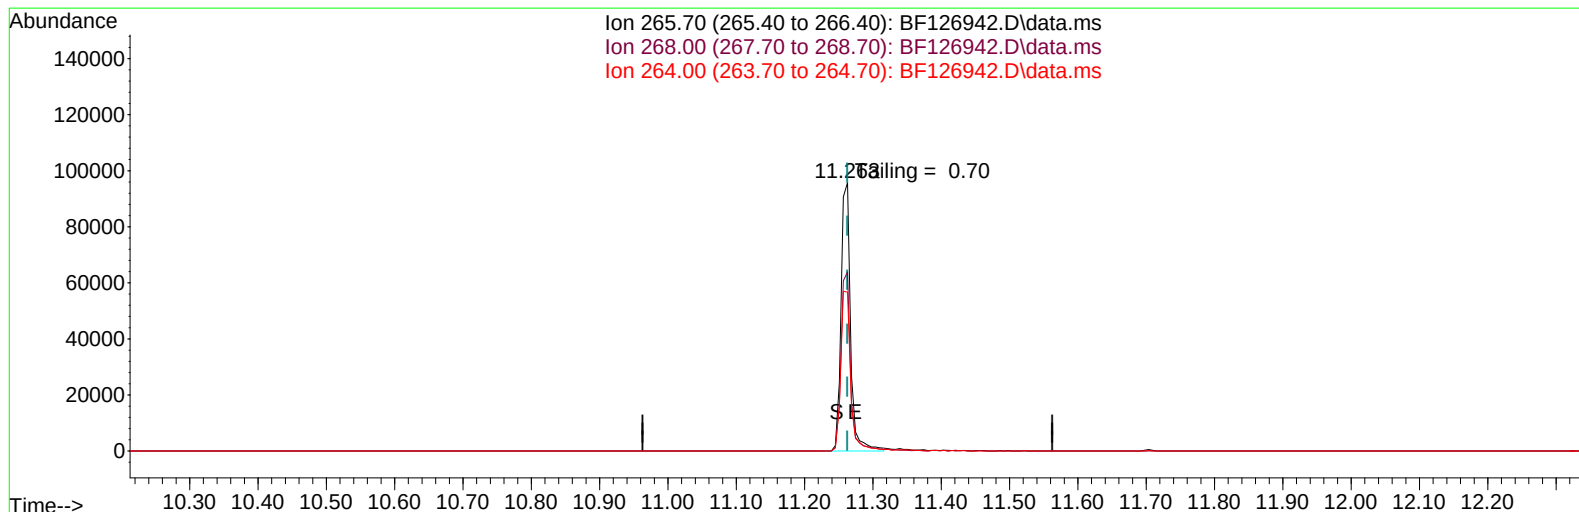

TIC: BF126942.D\data.ms

**(70) Pentachlorophenol (C)**

11.263min (+ 0.000) 29147.29 ng

response 92628

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.40  | 66.74  |
| 264.00 | 63.00  | 59.18  |
| 0.00   | 0.00   | 0.00   |