
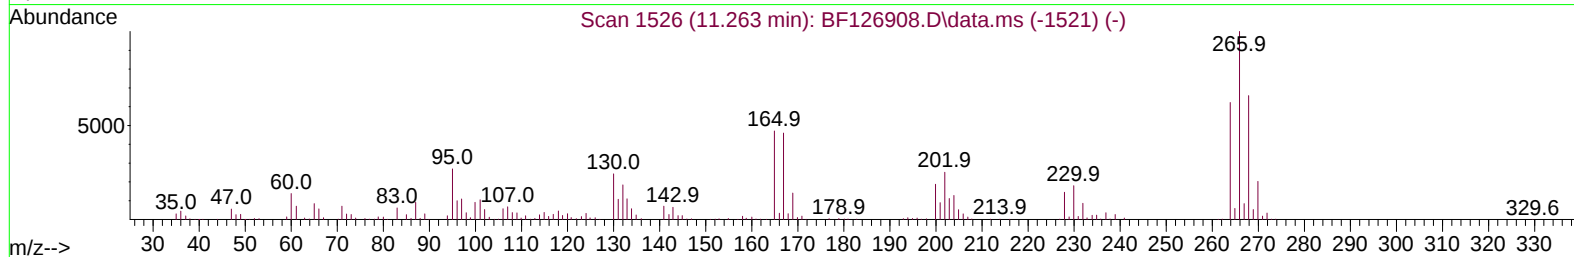
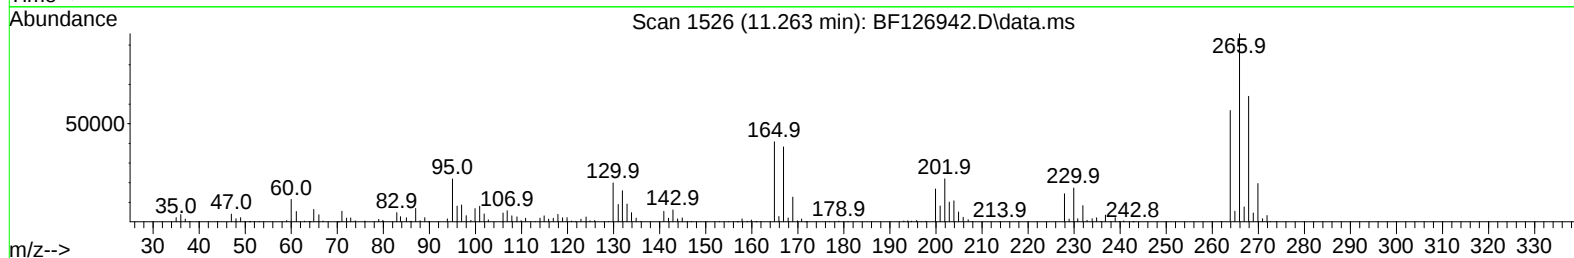


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126942.D
Acq On : 18 Feb 2022 09:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 16:06:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

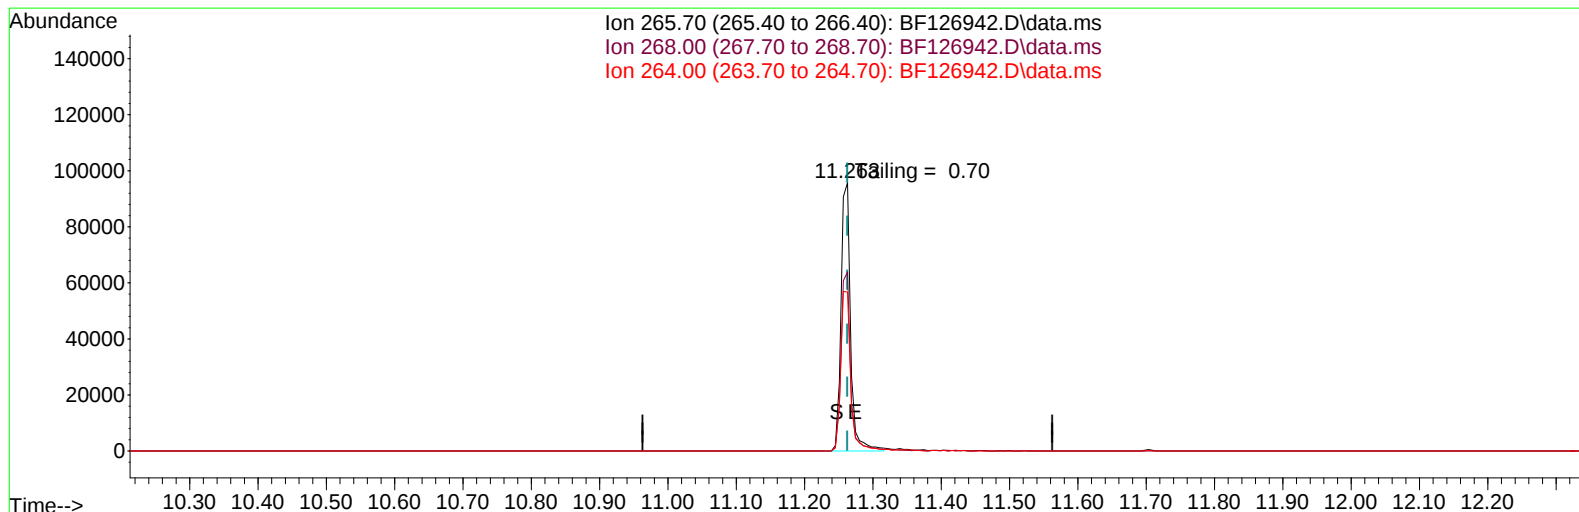

TIC: BF126942.D\data.ms

(70) Pentachlorophenol (C)




11.263min (+ 0.000) 29147.29 ng

response 92628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.74
264.00	63.00	59.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126942.D
Acq On : 18 Feb 2022 09:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 16:06:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

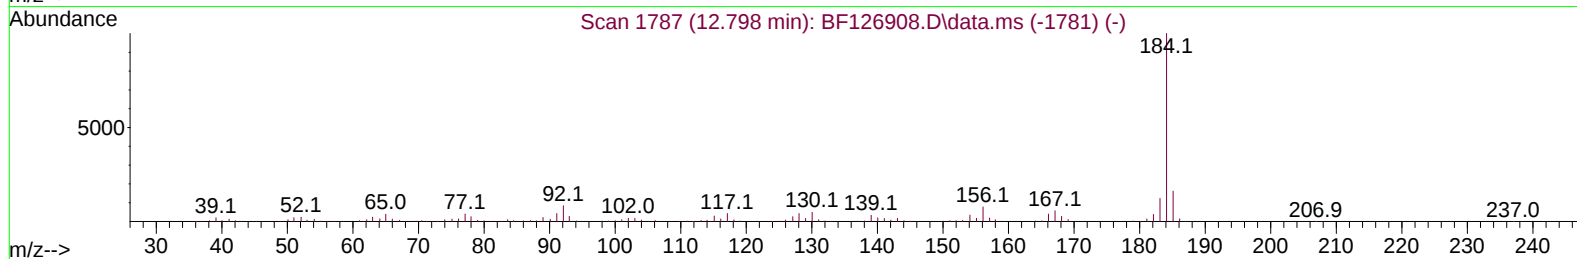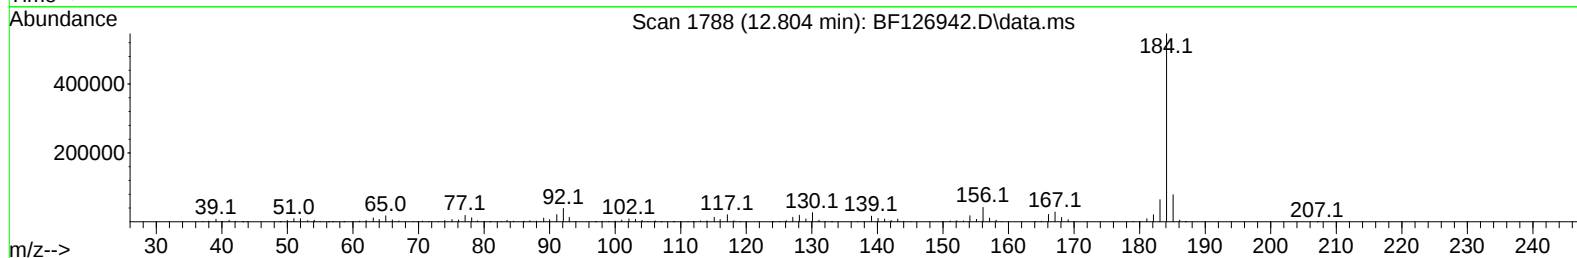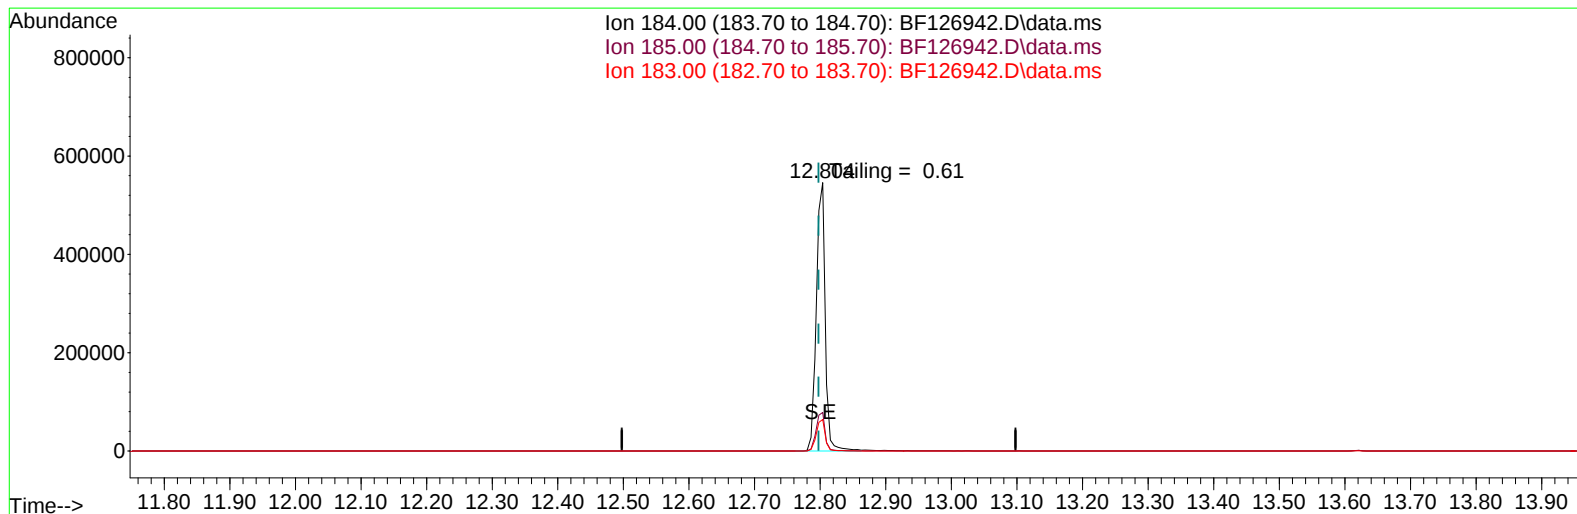

TIC: BF126942.D\data.ms

(77) Benzidine

12.804min (+ 0.006) 0.00 ng

response 516155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.41
183.00	10.20	11.79
0.00	0.00	0.00