

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
 Data File : BF126947.D
 Acq On : 18 Feb 2022 12:15
 Operator : CG\JU
 Sample : PB142738BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142738BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126947.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	551	556	559	rBV	3073164	3151838	76.42%	13.194%
2	6.551	719	725	728	rBV	2738027	3228995	78.29%	13.517%
3	6.928	786	789	793	rVB	830242	651760	15.80%	2.728%
4	7.492	879	885	888	rBV	2067772	2209005	53.56%	9.247%
5	8.210	1002	1007	1011	rBV	1010636	878582	21.30%	3.678%
6	9.286	1184	1190	1193	rBV	3971627	3770074	91.41%	15.782%
7	9.969	1302	1306	1309	rBV	1225840	956160	23.18%	4.003%
8	10.763	1436	1441	1444	rBV	2693500	2447944	59.35%	10.248%
9	11.457	1556	1559	1563	rBV	1102387	999657	24.24%	4.185%
10	12.857	1793	1797	1800	rBV	72357	56210	1.36%	0.235%
11	13.051	1825	1830	1833	rBV	4479836	4124324	100.00%	17.265%
12	14.104	2005	2009	2016	rBV	884937	764218	18.53%	3.199%
13	15.610	2259	2265	2279	rVB	491054	649222	15.74%	2.718%




Sum of corrected areas: 23887989

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126947.D
Acq On : 18 Feb 2022 12:15
Operator : CG\JU
Sample : PB142738BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

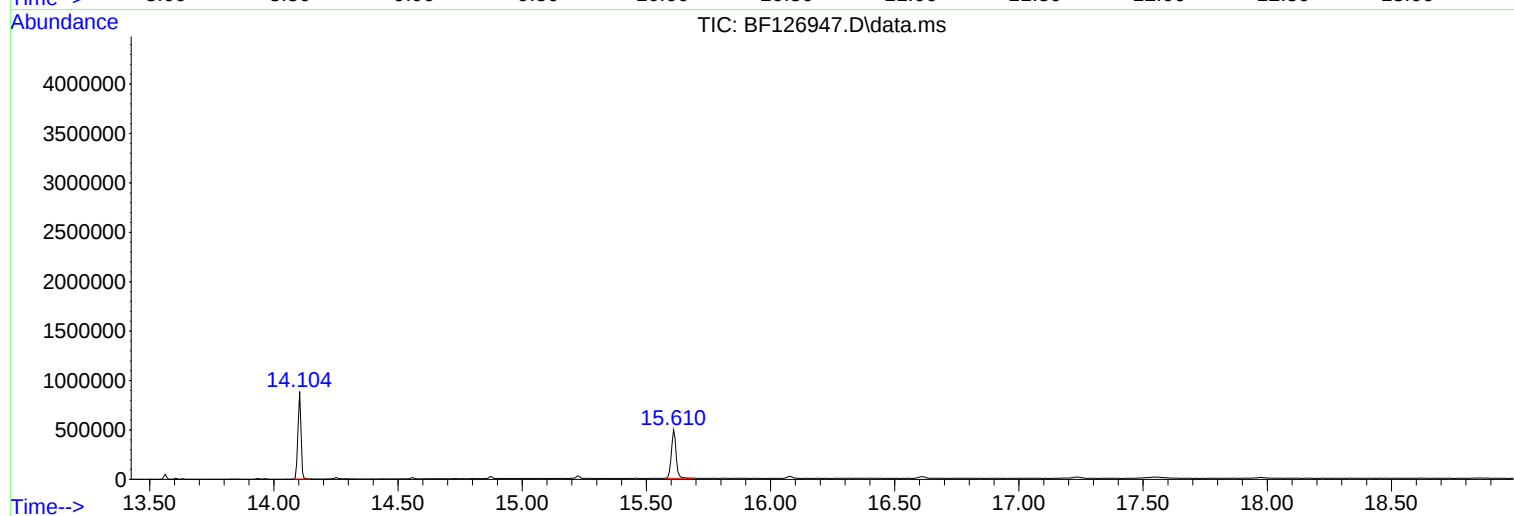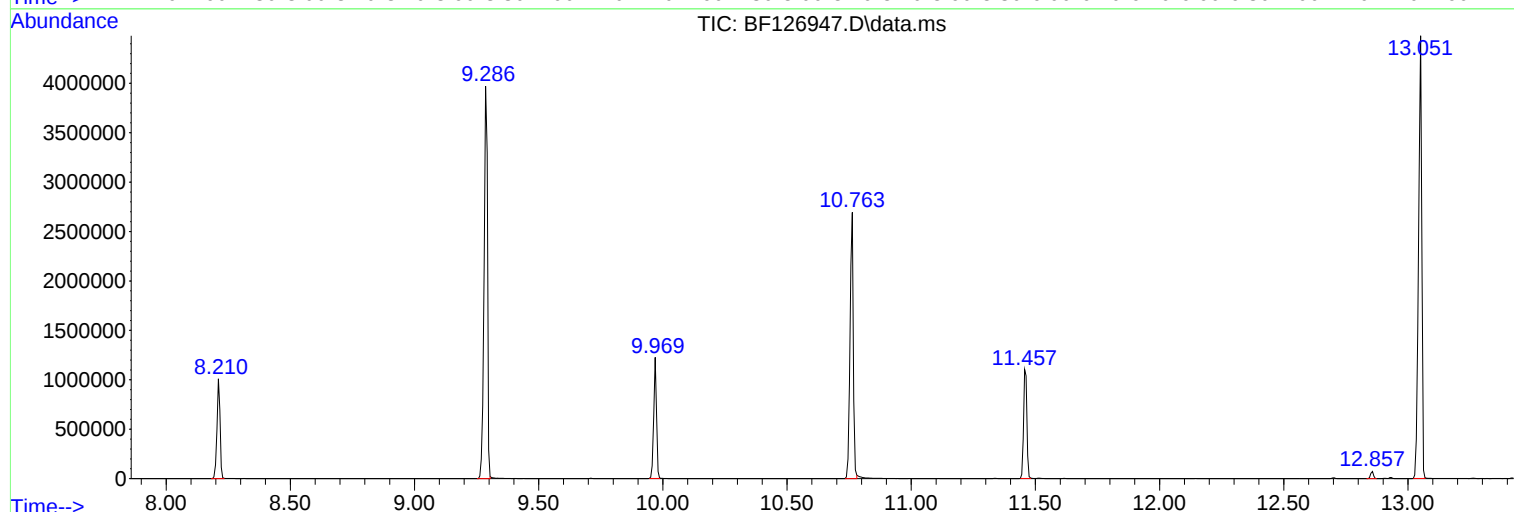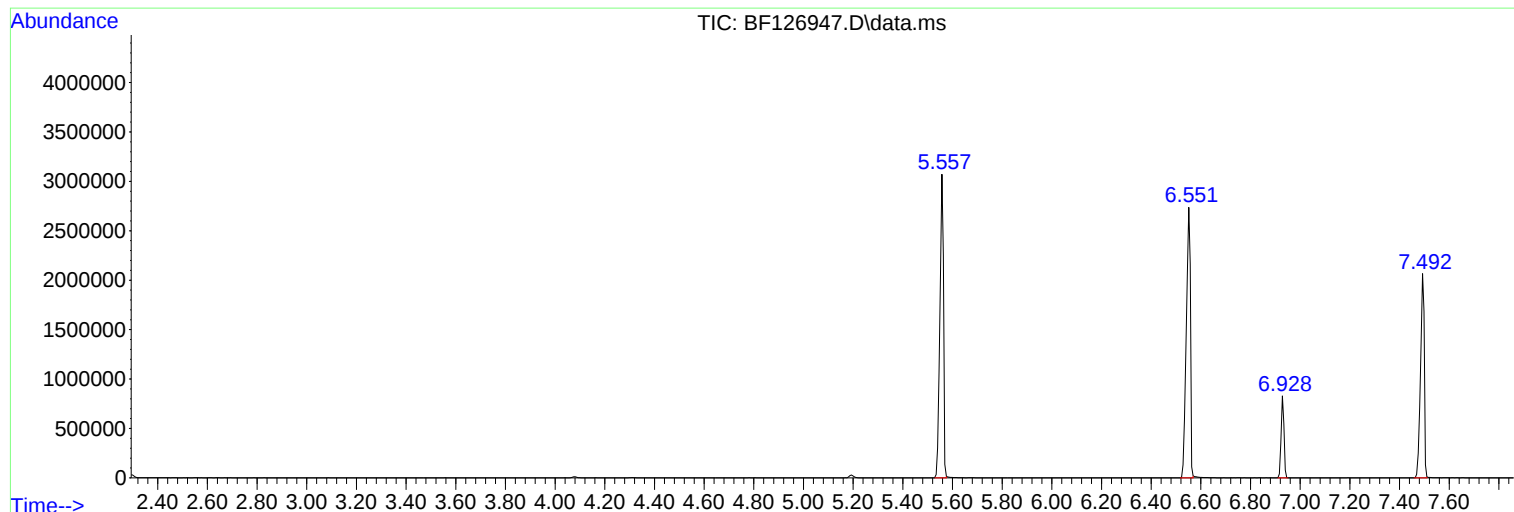

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126947.D
Acq On : 18 Feb 2022 12:15
Operator : CG\JU
Sample : PB142738BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126947.D
Acq On : 18 Feb 2022 12:15
Operator : CG\JU
Sample : PB142738BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142738BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------