

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
 Data File : BF126948.D
 Acq On : 18 Feb 2022 12:44
 Operator : CG\JU
 Sample : PB142712BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142712BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.557	551	556	559	rBV	3060145	3147363	76.91%	13.206%
2	6.551	719	725	728	rBV	2774500	3221825	78.73%	13.518%
3	6.928	786	789	793	rVB	836951	648920	15.86%	2.723%
4	7.493	879	885	888	rBV	2026106	2216915	54.17%	9.302%
5	8.210	1002	1007	1011	rBV	1040509	879105	21.48%	3.688%
6	9.287	1184	1190	1193	rBV	4016798	3805911	93.00%	15.969%
7	9.969	1302	1306	1309	rBV	1202599	954344	23.32%	4.004%
8	10.763	1436	1441	1444	rBV	2679586	2439289	59.61%	10.235%
9	11.457	1556	1559	1563	rBV	1098369	1019103	24.90%	4.276%
10	12.857	1793	1797	1800	rBV	77975	60379	1.48%	0.253%
11	13.051	1825	1830	1833	rBV	4459678	4092231	100.00%	17.170%
12	14.104	2005	2009	2012	rBV	853963	740660	18.10%	3.108%
13	15.610	2259	2265	2274	rBV	463532	607682	14.85%	2.550%




Sum of corrected areas: 23833727

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126948.D
Acq On : 18 Feb 2022 12:44
Operator : CG\JU
Sample : PB142712BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

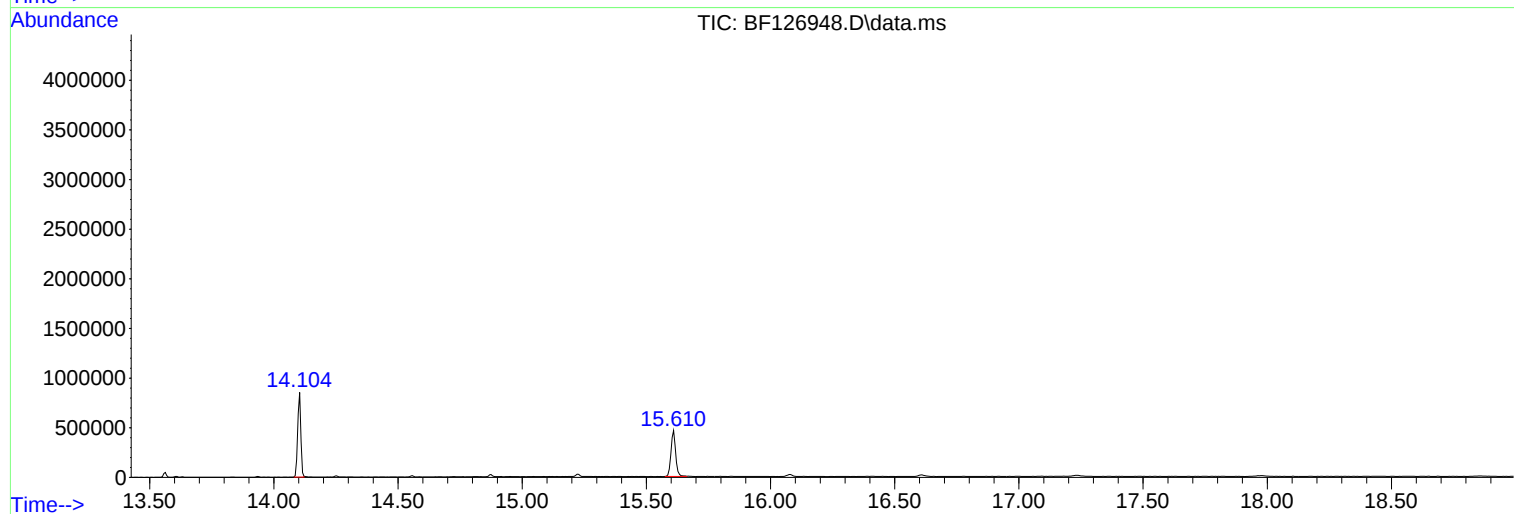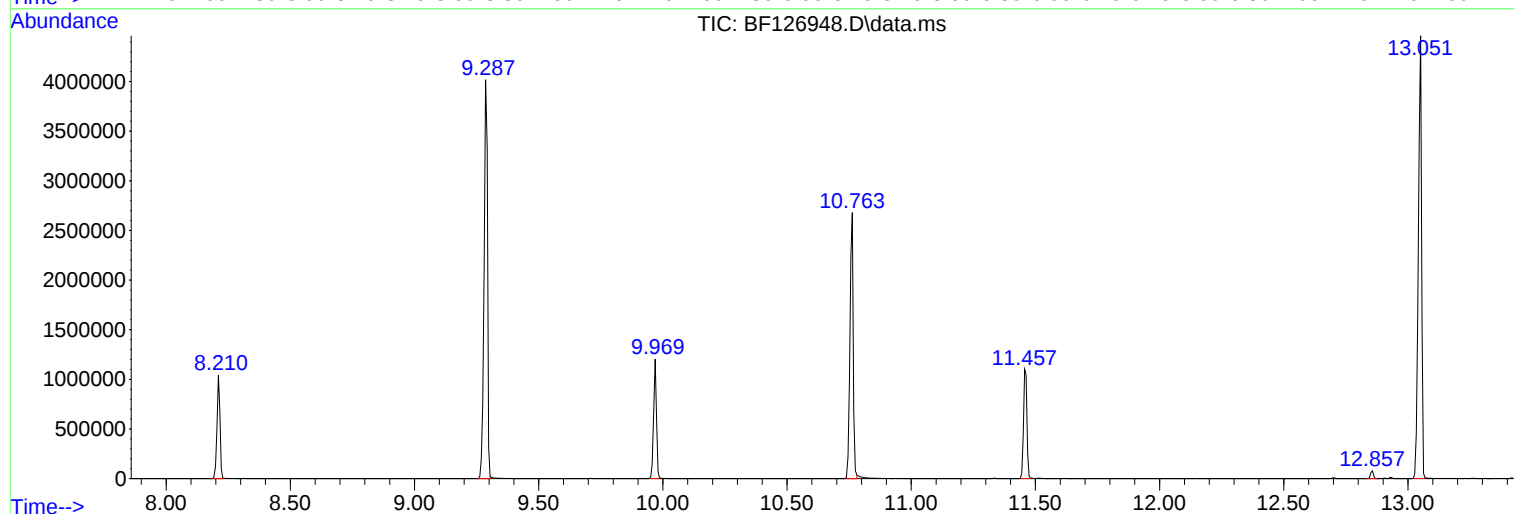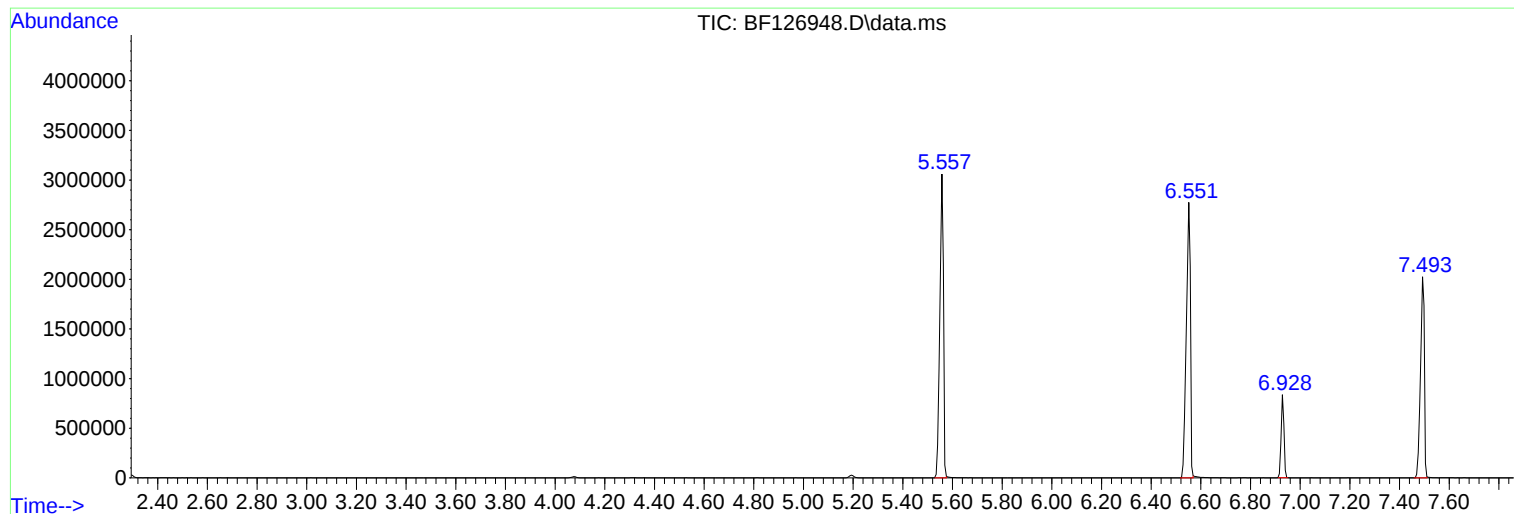

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126948.D
Acq On : 18 Feb 2022 12:44
Operator : CG\JU
Sample : PB142712BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126948.D
Acq On : 18 Feb 2022 12:44
Operator : CG\JU
Sample : PB142712BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142712BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------