

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
 Data File : BF126954.D
 Acq On : 18 Feb 2022 16:11
 Operator : CG\JU
 Sample : PB142473BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB142473BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF126954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.563	551	557	560	rBV	3289118	3356568	71.53%	12.517%
2	6.557	719	726	729	rBV	2978835	3434046	73.18%	12.806%
3	6.928	785	789	793	rBV	901735	692725	14.76%	2.583%
4	7.492	879	885	888	rBV	2139283	2380743	50.74%	8.878%
5	8.210	1002	1007	1011	rBV	1030480	947282	20.19%	3.533%
6	9.286	1184	1190	1193	rBV	4050929	4096089	87.29%	15.275%
7	9.969	1301	1306	1309	rBV	1261816	1037300	22.11%	3.868%
8	10.763	1435	1441	1444	rBV	3013214	2771773	59.07%	10.336%
9	11.463	1555	1560	1563	rBV	1300436	1119317	23.85%	4.174%
10	12.857	1794	1797	1800	rVB	125168	94254	2.01%	0.351%
11	13.057	1825	1831	1833	rBV	4418636	4692366	100.00%	17.498%
12	13.563	1908	1917	1921	rBV	97553	87757	1.87%	0.327%
13	13.939	1968	1981	1983	rBV2	50005	105371	2.25%	0.393%
14	14.104	1999	2009	2013	rBV	1041779	997133	21.25%	3.718%
15	15.227	2196	2200	2205	rBV	44092	51827	1.10%	0.193%
16	15.615	2260	2266	2274	rBV	615328	814600	17.36%	3.038%
17	16.080	2340	2345	2350	rBV2	42693	66144	1.41%	0.247%
18	16.609	2430	2435	2443	rVB2	39413	70657	1.51%	0.263%




Sum of corrected areas: 26815952

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126954.D
Acq On : 18 Feb 2022 16:11
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

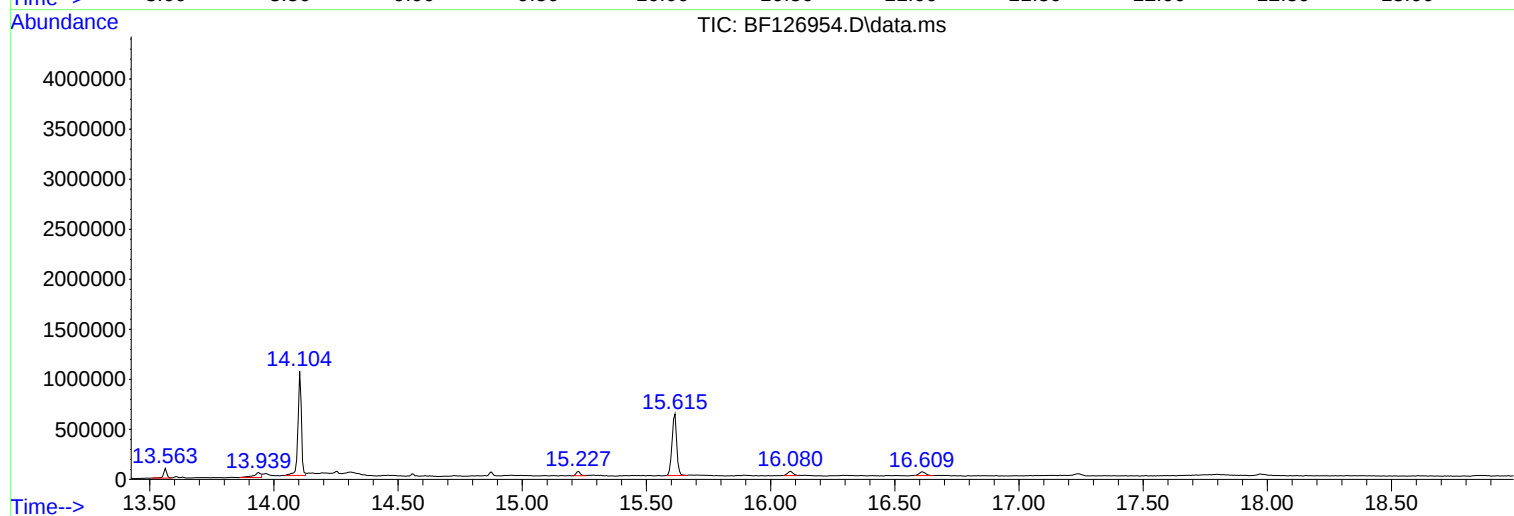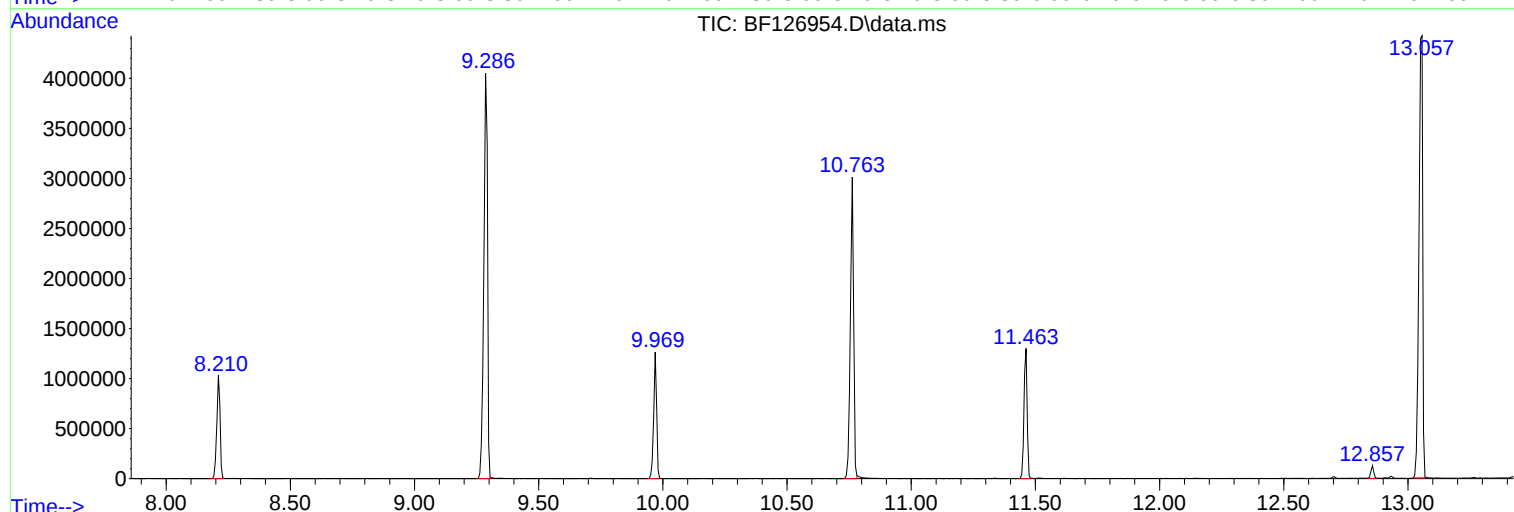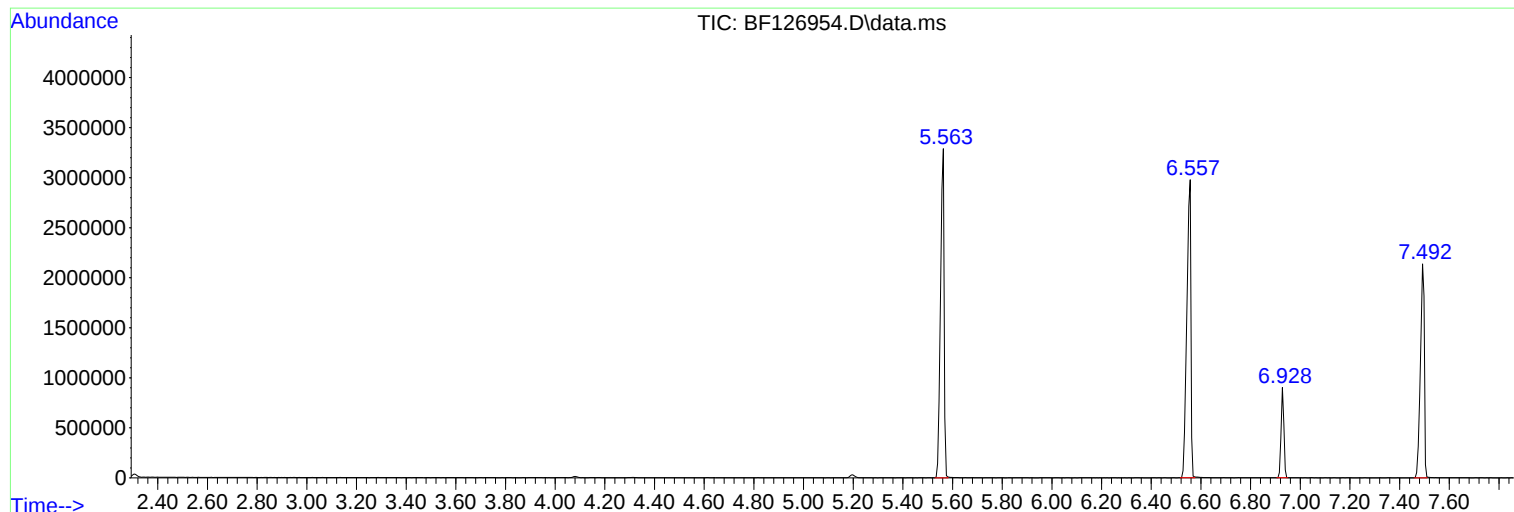

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126954.D
Acq On : 18 Feb 2022 16:11
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Ethanol, 2-(hexadecyloxy)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.939	2.11 ng	105371	Chrysene-d12	14.104

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Ethanol, 2-(hexadecyloxy)-	286	C18H38O2	002136-71-2	74
2			Carbonic acid, octadecyl prop-1-...	354	C22H42O3	1000383-11-5	68
3			Carbonic acid, hexadecyl prop-1-...	326	C20H38O3	1000382-90-3	68
4			Oxalic acid, isobutyl tetradecyl...	342	C20H38O4	1000309-37-9	64
5			Oxalic acid, isobutyl pentadecyl...	356	C21H40O4	1000309-38-0	64

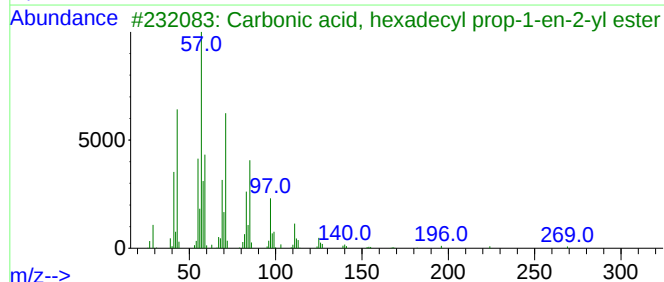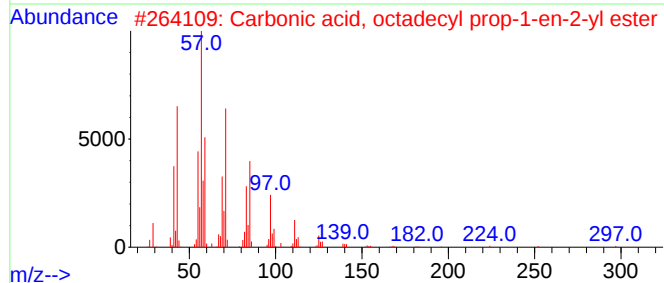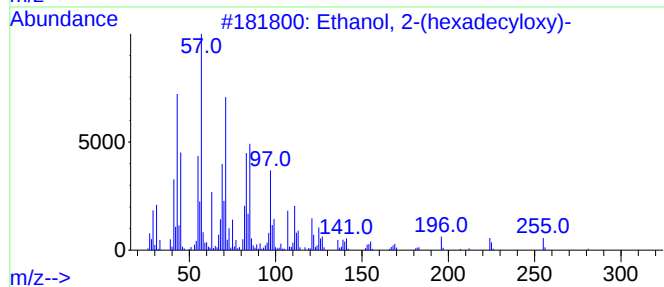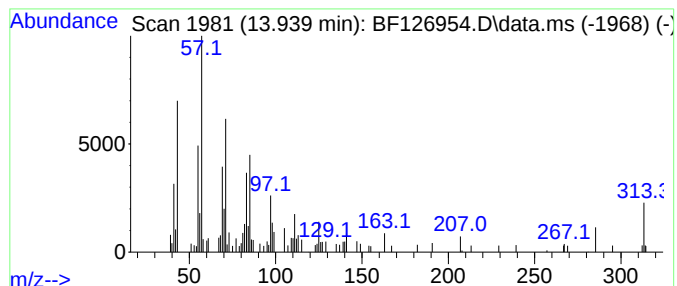

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126954.D
Acq On : 18 Feb 2022 16:11
Operator : CG\JU
Sample : PB142473BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB142473BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Ethanol, 2-(hex...	13.939	2.1	ng	105371	5	14.104	997133	20.0