


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
 Data File : BF126942.D
 Acq On : 18 Feb 2022 09:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Feb 21 13:16:57 2022

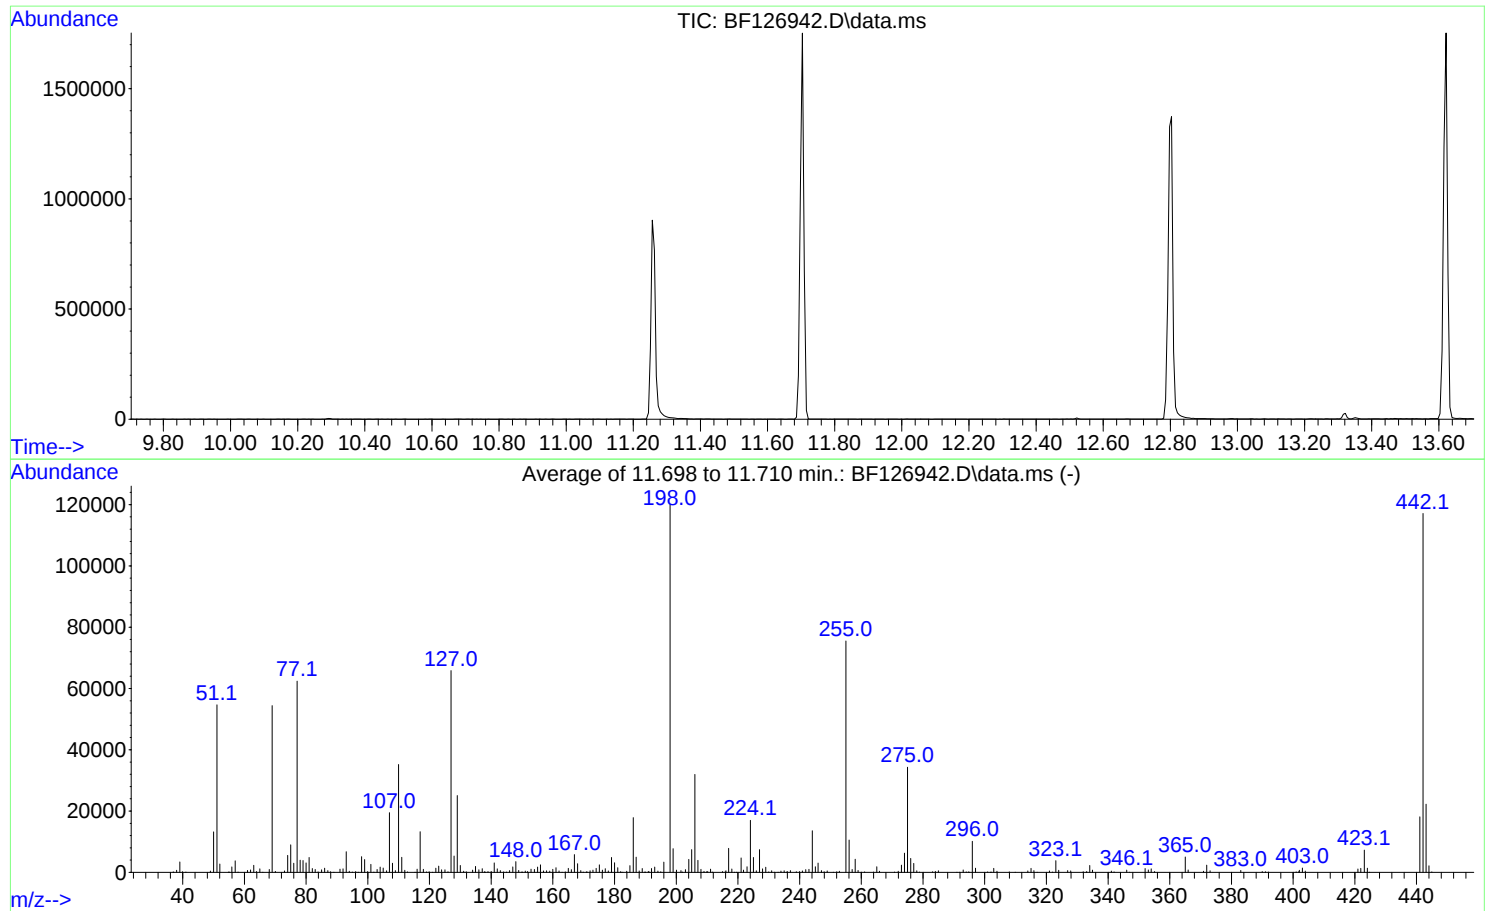




AutoFind: Scans 1600, 1601, 1602; Background Corrected with Scan 1595

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.5	54680	PASS
68	69	0.00	2	1.7	946	PASS
69	198	0.00	100	45.3	54429	PASS
70	69	0.00	2	0.6	306	PASS
127	198	10	80	54.8	65824	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	120045	PASS
199	198	5	9	6.4	7728	PASS
275	198	10	60	28.6	34317	PASS
365	198	1	100	4.2	5030	PASS
441	198	0.01	100	15.1	18124	PASS
442	442	50	100	100.0	117128	PASS
443	442	15	24	19.0	22266	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
 Data File : BF126942.D
 Acq On : 18 Feb 2022 09:52
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 18 16:06:38 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Feb 16 14:55:48 2022
 Response via : Initial Calibration

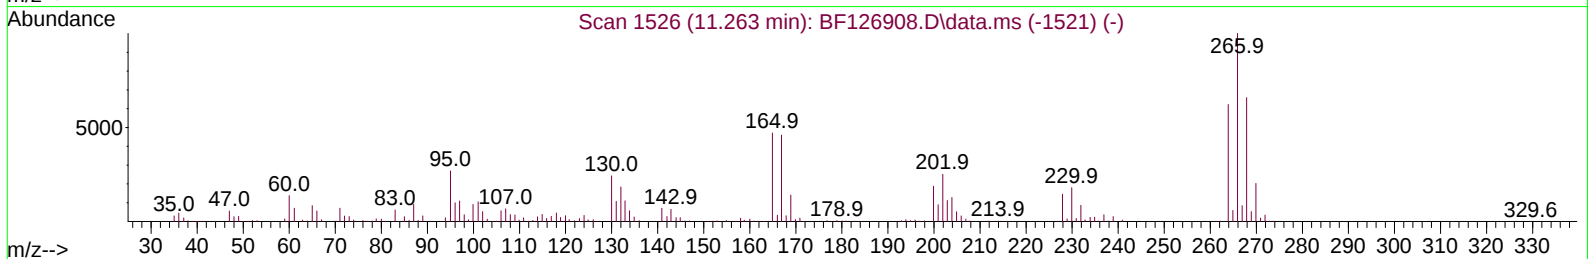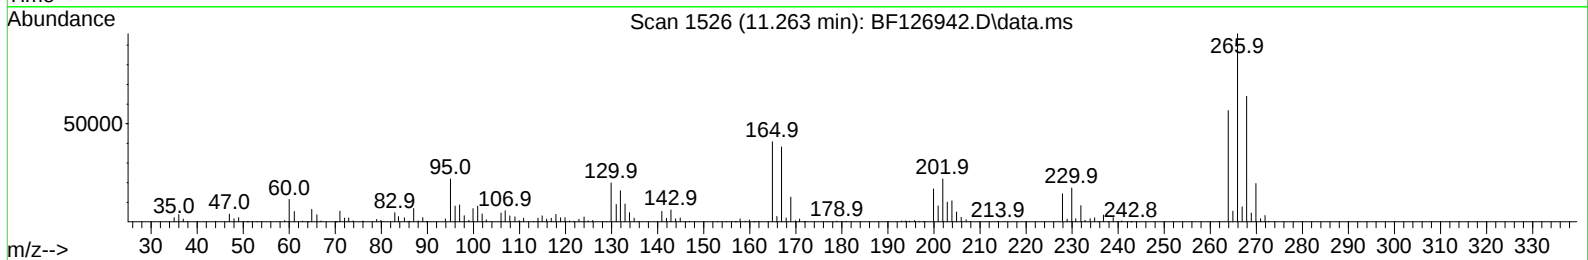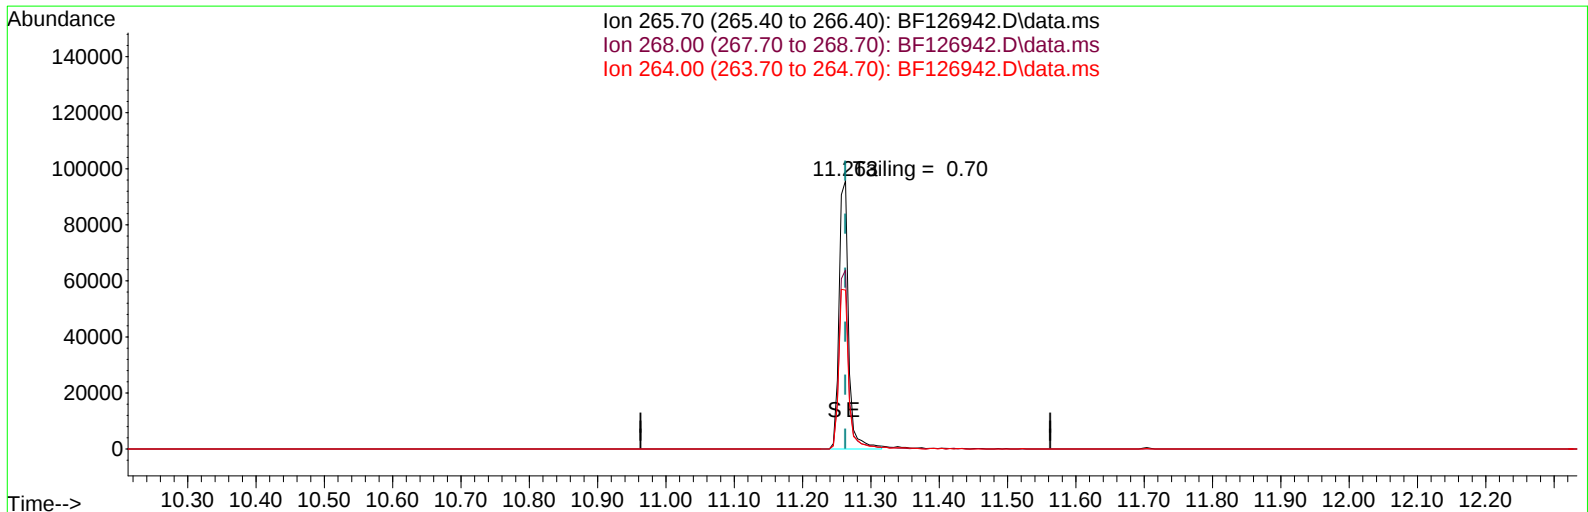

TIC: BF126942.D\data.ms

(70) Pentachlorophenol (C)

11.263min (+ 0.000) 29147.29 ng




response 92628

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	66.74
264.00	63.00	59.18
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021822\
Data File : BF126942.D
Acq On : 18 Feb 2022 09:52
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 16:06:38 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Feb 16 14:55:48 2022
Response via : Initial Calibration

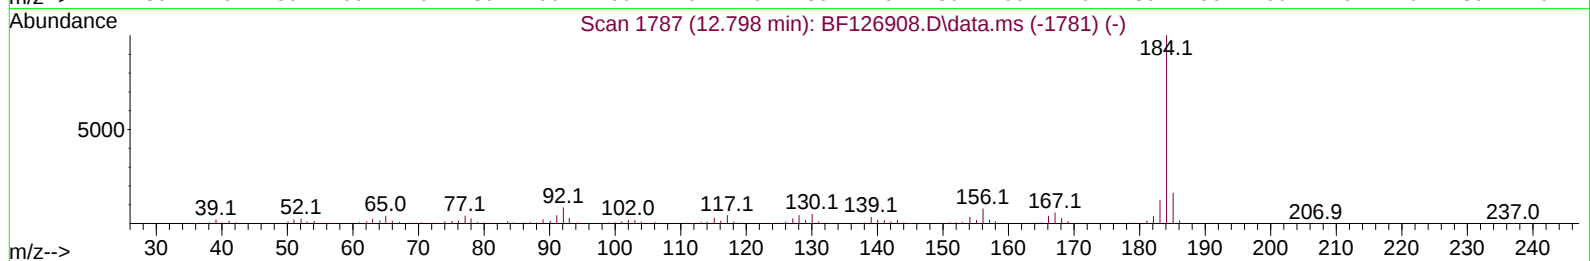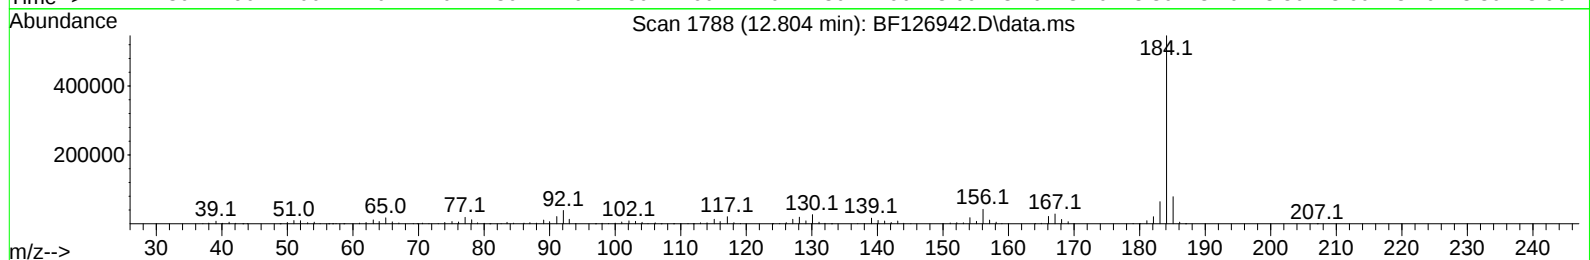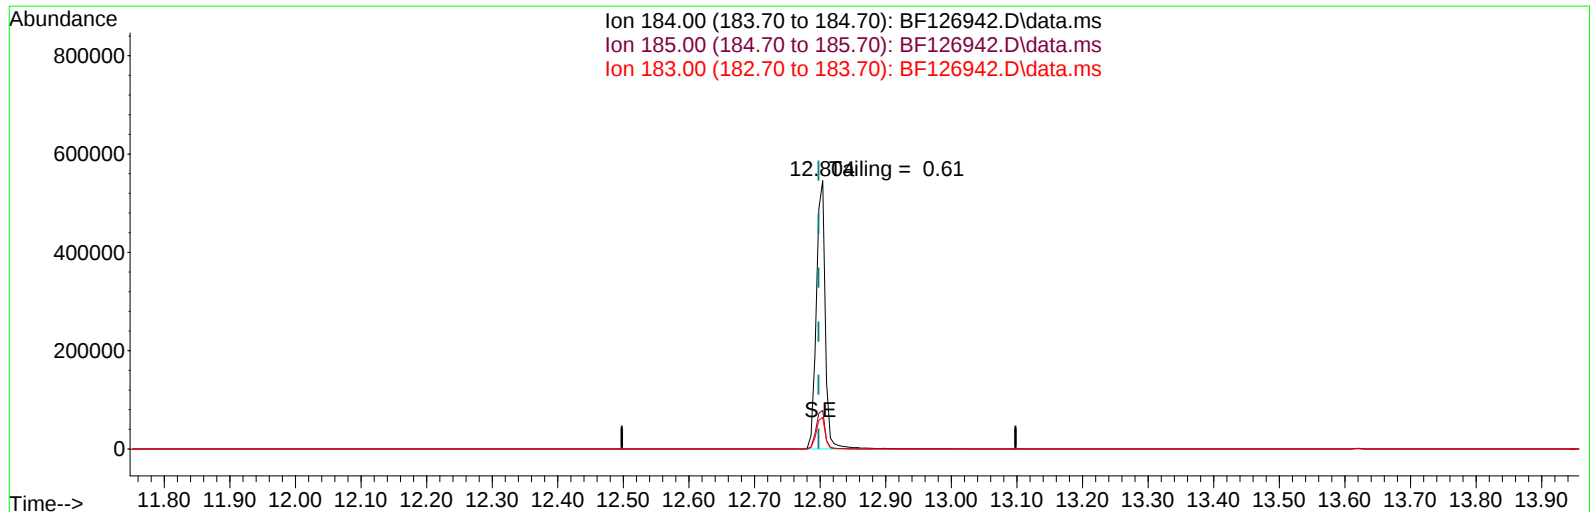

TIC: BF126942.D\data.ms

(77) Benzidine

12.804min (+ 0.006) 0.00 ng

response 516155

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.41
183.00	10.20	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/18/2022	BNA_F	<u>BF126942.D</u>
Compound Name	Response	Retention Time
DDT	255182	13.62
DDD	4157	13.32
DDE	408	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4565	259747	1.76

Instrument :
BNA_F
ClientSampleId :
DFTPP