
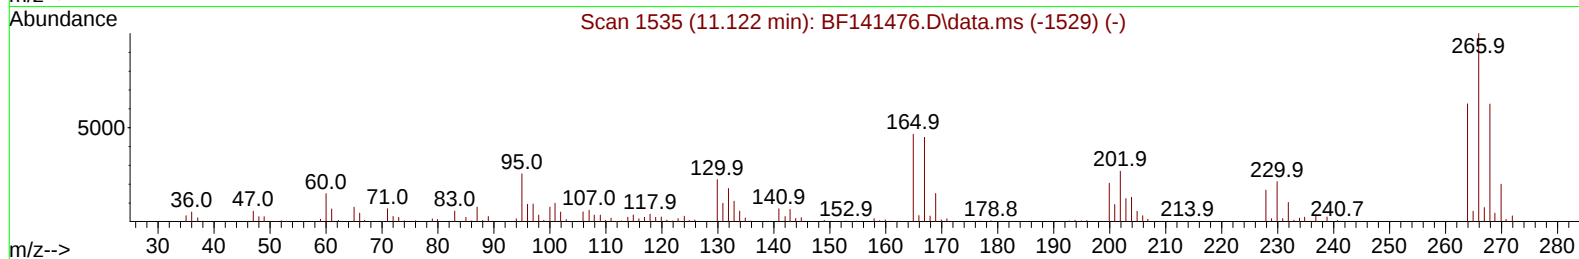
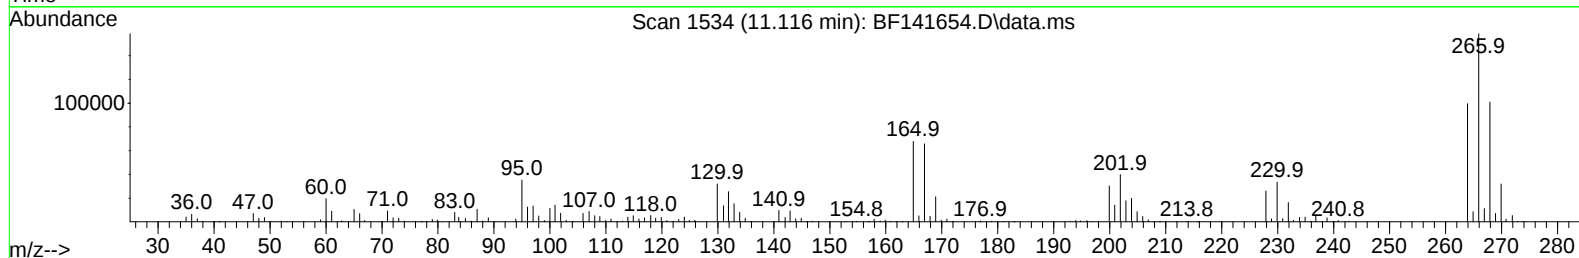


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141654.D
Acq On : 18 Feb 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

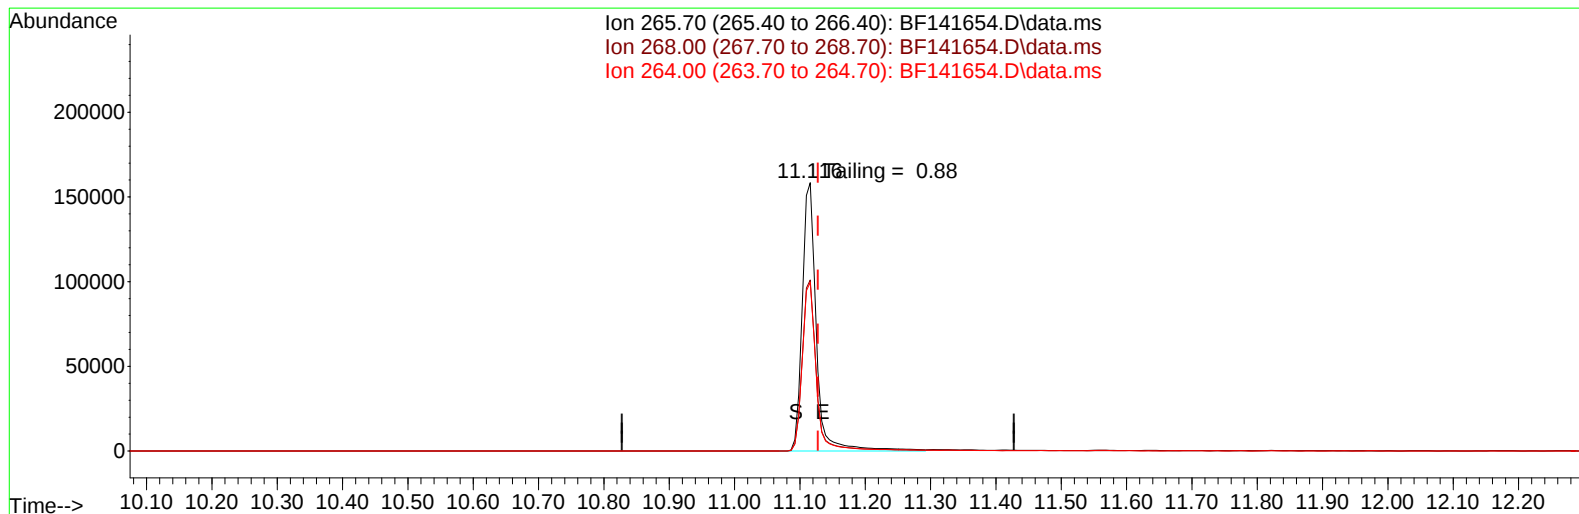

TIC: BF141654.D\data.ms

(70) Pentachlorophenol (C)




11.116min (-0.012) 60529.65 ng

response 238303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.72
264.00	62.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141654.D
Acq On : 18 Feb 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

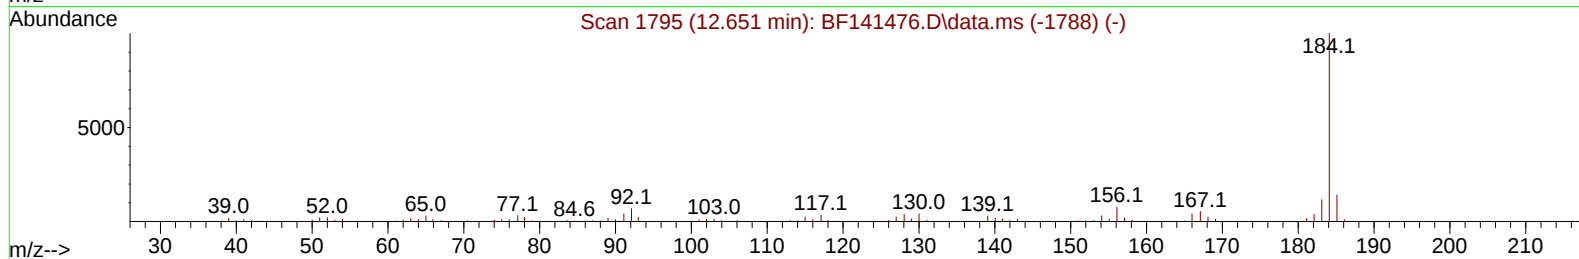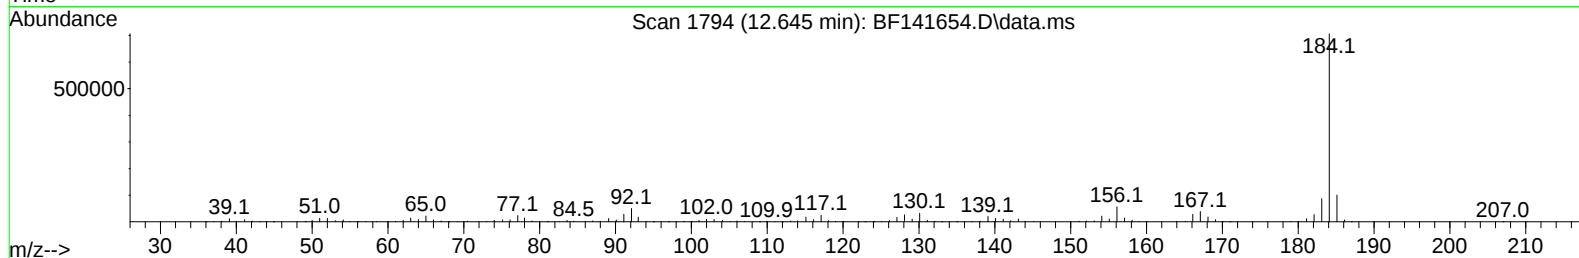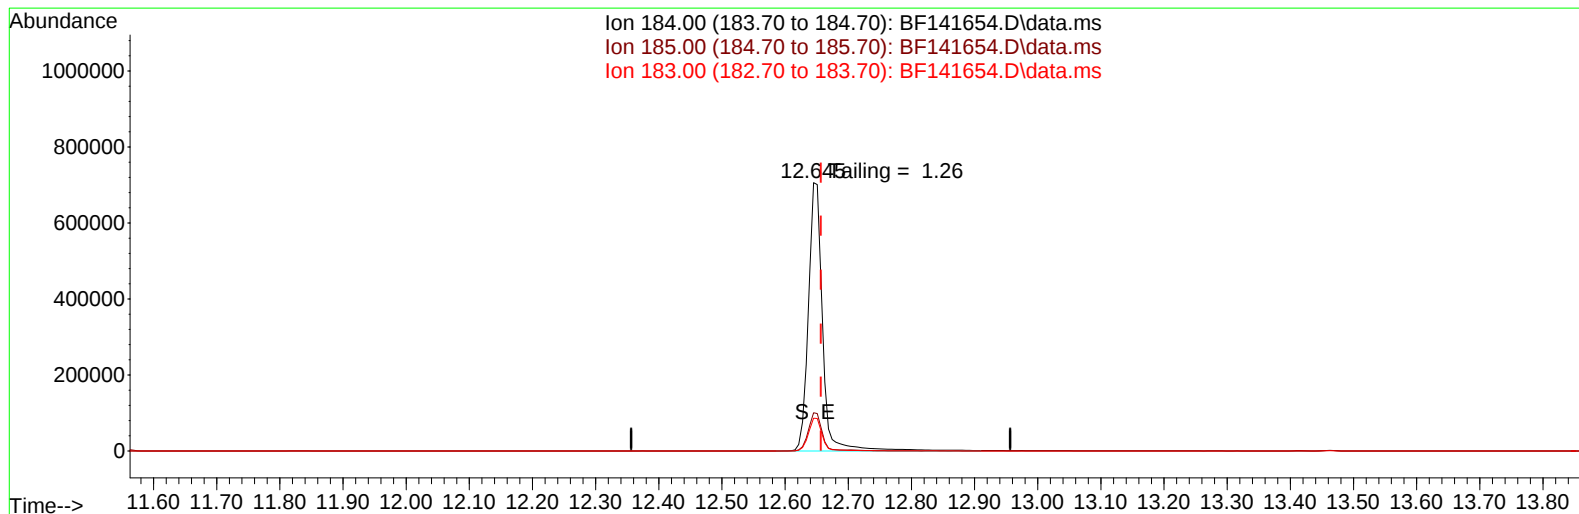

TIC: BF141654.D\data.ms

(77) Benzidine

12.645min (-0.012) 15778.91 ng

response 1110447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.26
183.00	11.60	12.24
0.00	0.00	0.00