

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
 Data File : BF141658.D
 Acq On : 18 Feb 2025 13:24
 Operator : RC/JU
 Sample : PB166751BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB166751BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141658.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.410	558	564	586	rBV	2151376	2917455	74.17%	13.197%
2	6.422	730	736	765	rBV	2041773	2941111	74.77%	13.304%
3	6.775	792	796	807	rBV	446335	588780	14.97%	2.663%
4	7.345	886	893	932	rBV	1314310	1965510	49.97%	8.891%
5	8.063	1008	1015	1032	rBV	535850	775835	19.72%	3.509%
6	9.139	1191	1198	1228	rBV	2550336	3601420	91.55%	16.290%
7	9.816	1306	1313	1331	rVB	654830	899203	22.86%	4.067%
8	10.604	1441	1447	1471	rBV	1601376	2177558	55.36%	9.850%
9	11.298	1560	1565	1593	rVB	665134	938120	23.85%	4.243%
10	12.892	1829	1836	1841	rBV	2789998	3933661	100.00%	17.793%
11	13.939	2008	2014	2025	rBV	576811	785966	19.98%	3.555%
12	15.380	2253	2259	2275	rBV	345711	582897	14.82%	2.637%




Sum of corrected areas: 22107516

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141658.D
Acq On : 18 Feb 2025 13:24
Operator : RC/JU
Sample : PB166751BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166751BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

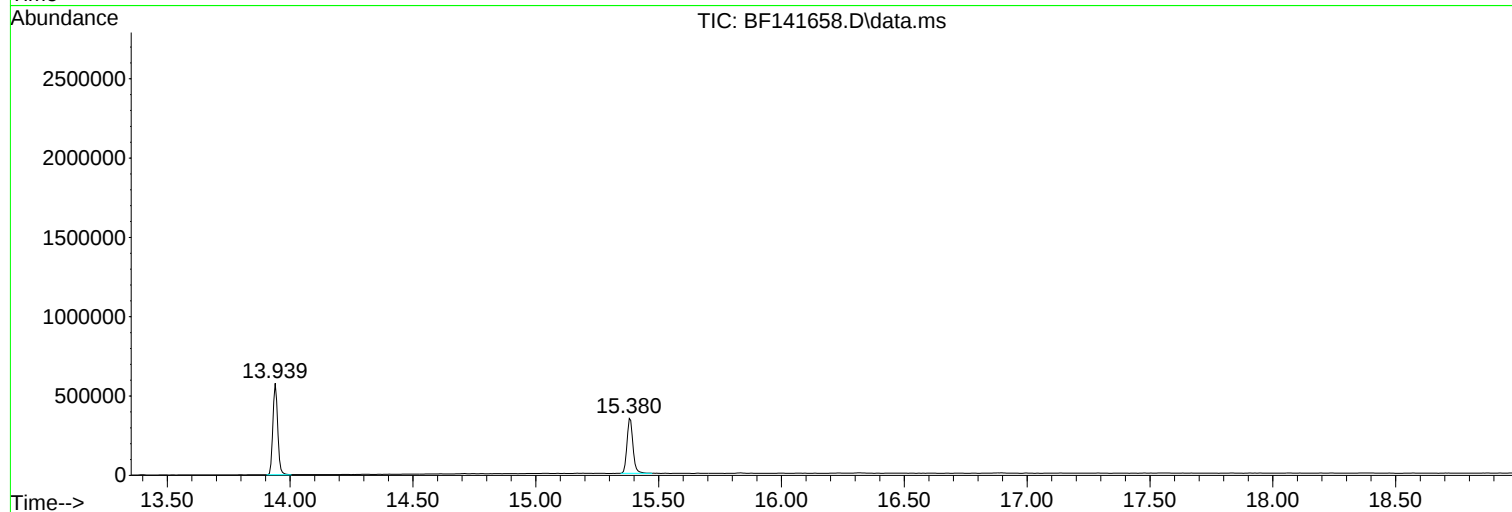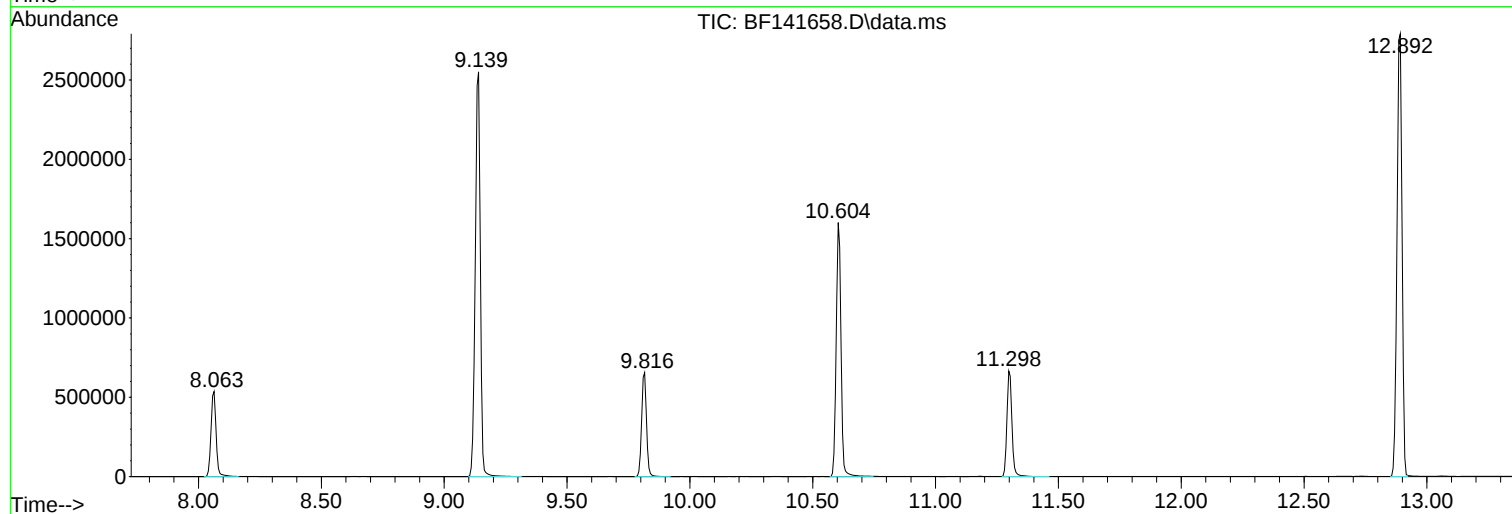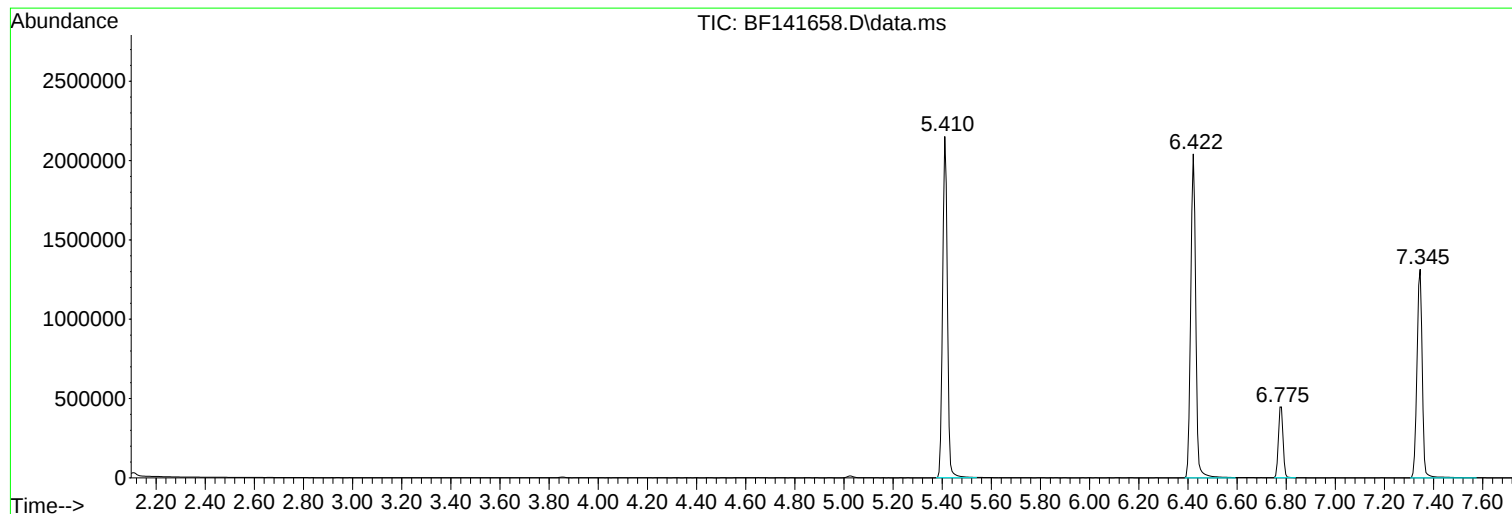

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141658.D
Acq On : 18 Feb 2025 13:24
Operator : RC/JU
Sample : PB166751BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166751BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141658.D
Acq On : 18 Feb 2025 13:24
Operator : RC/JU
Sample : PB166751BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB166751BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------