


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141654.D
Acq On : 18 Feb 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Feb 06 16:58:59 2025

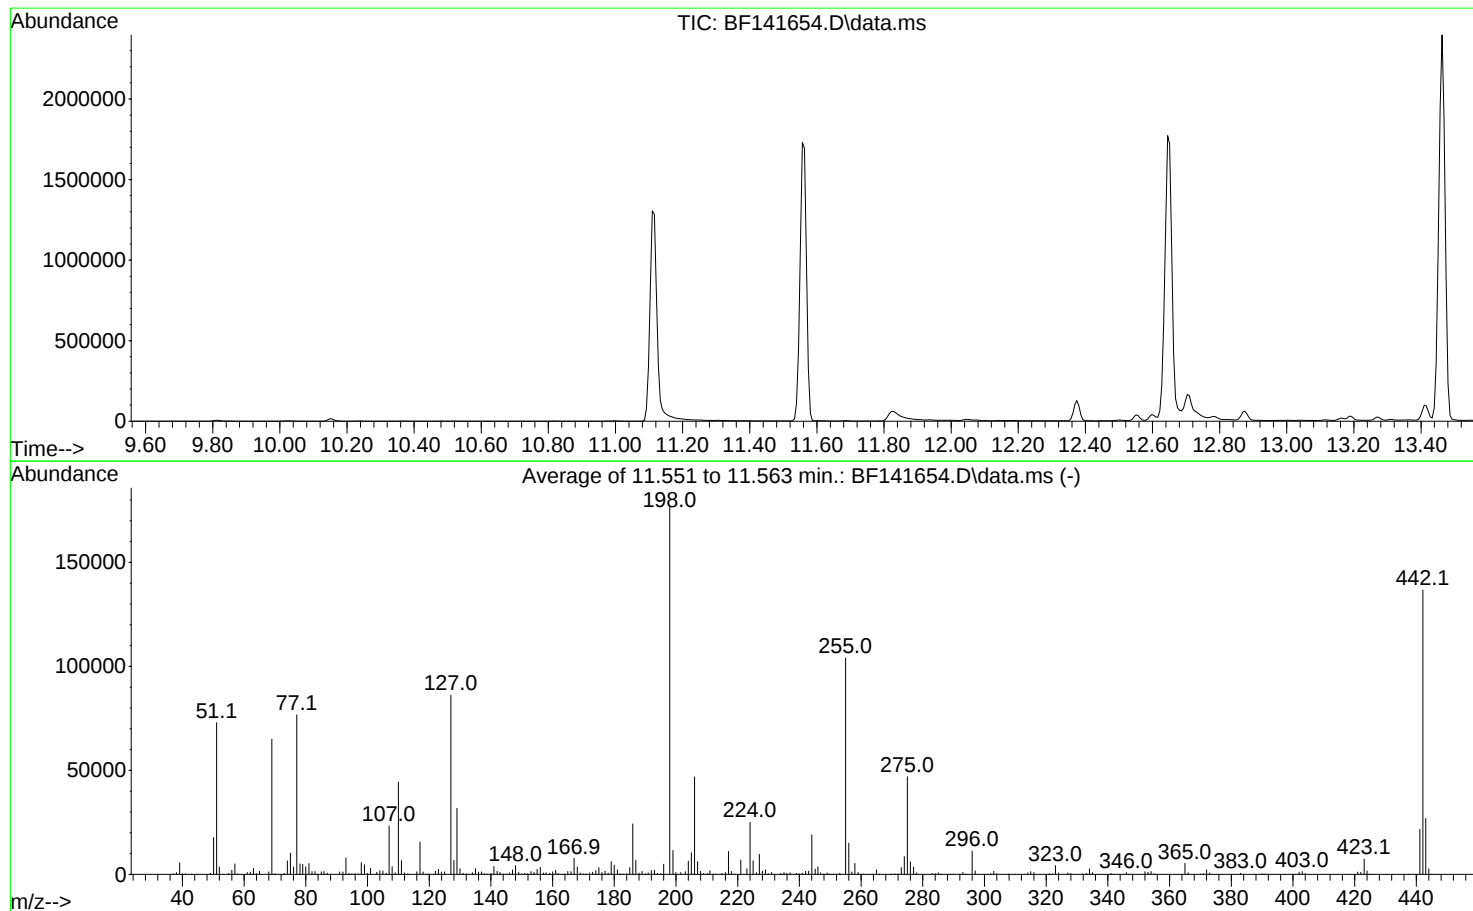

AutoFind: Scans 1608, 1609, 1610; Background Corrected with Scan 1602

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	72917	PASS
68	69	0.00	2	1.8	1181	PASS
69	198	0.00	100	36.8	65011	PASS
70	69	0.00	2	0.5	320	PASS
127	198	10	80	48.7	86123	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	176832	PASS
199	198	5	9	6.5	11486	PASS
275	198	10	60	26.5	46888	PASS
365	198	1	100	3.0	5274	PASS
441	198	0.01	100	12.2	21622	PASS
442	442	50	100	100.0	136661	PASS
443	442	15	24	19.7	26887	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
2/18/2025	BNA_F	<u>BF141654.D</u>
Compound Name	Response	Retention Time
DDT	624560	13.463
DDD	12458	13.192
DDE	606	12.827
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13064	637624	2.05

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141654.D
Acq On : 18 Feb 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

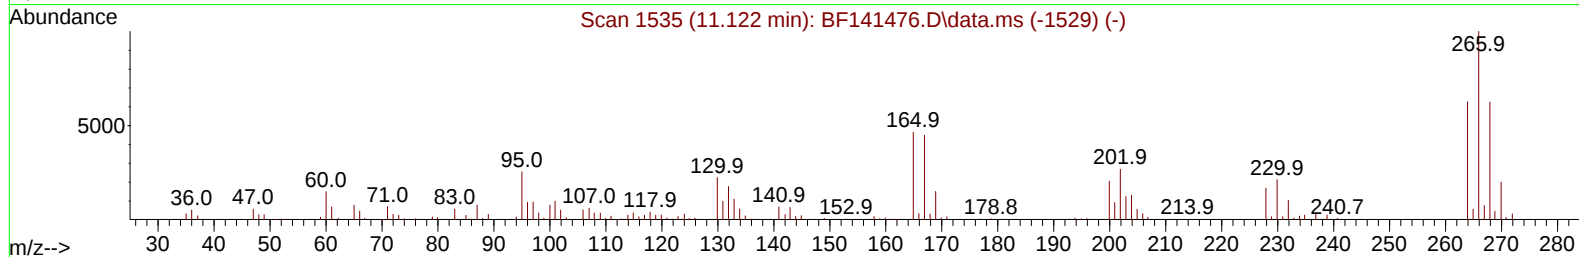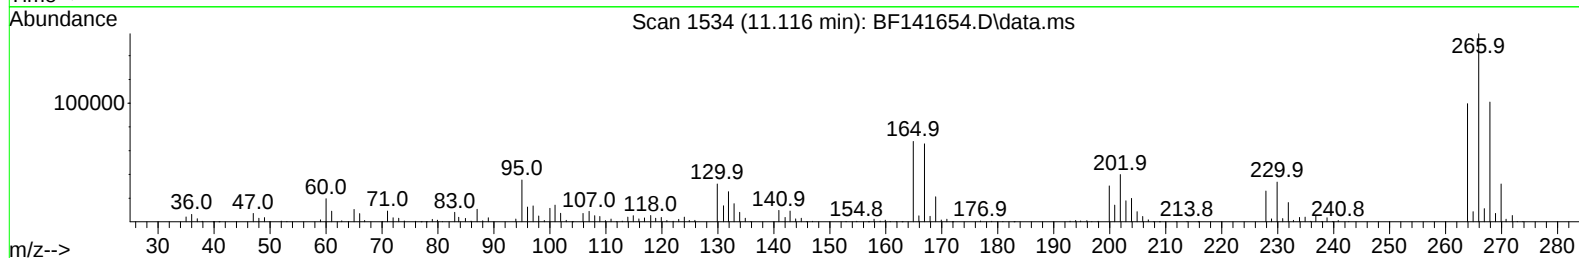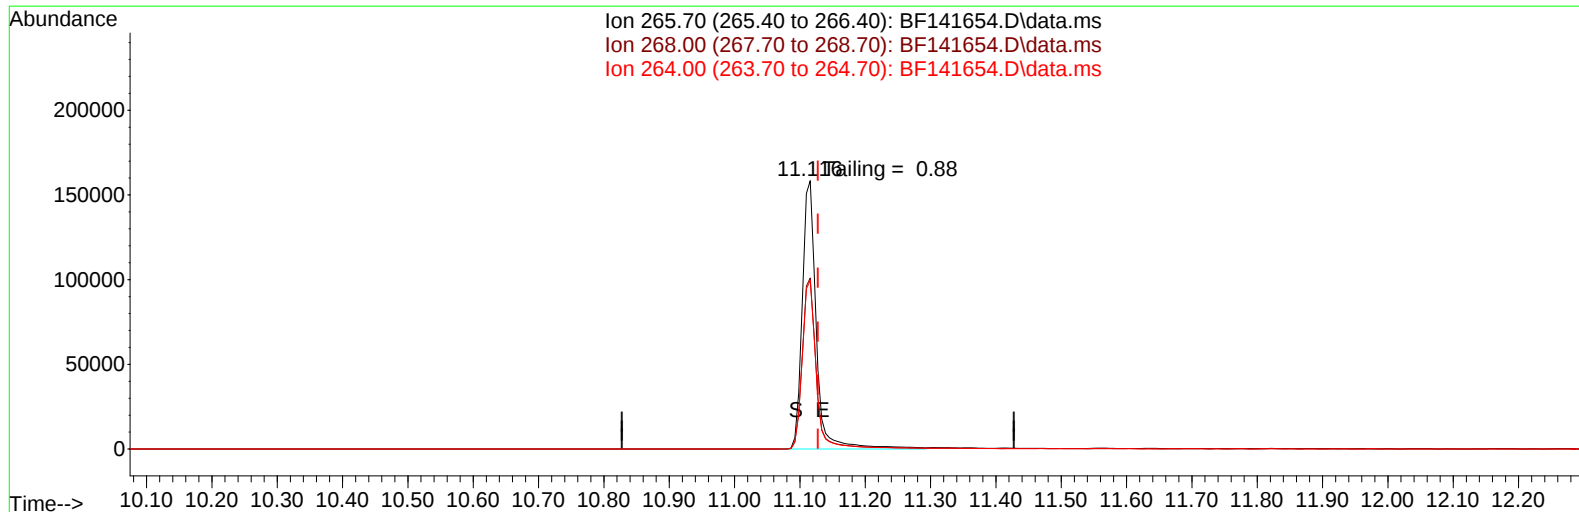

TIC: BF141654.D\data.ms

(70) Pentachlorophenol (C)

11.116min (-0.012) 60529.65 ng




response 238303

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.60	63.72
264.00	62.60	62.84
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021825\
Data File : BF141654.D
Acq On : 18 Feb 2025 08:53
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 18 10:50:54 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Feb 06 16:58:59 2025
Response via : Initial Calibration

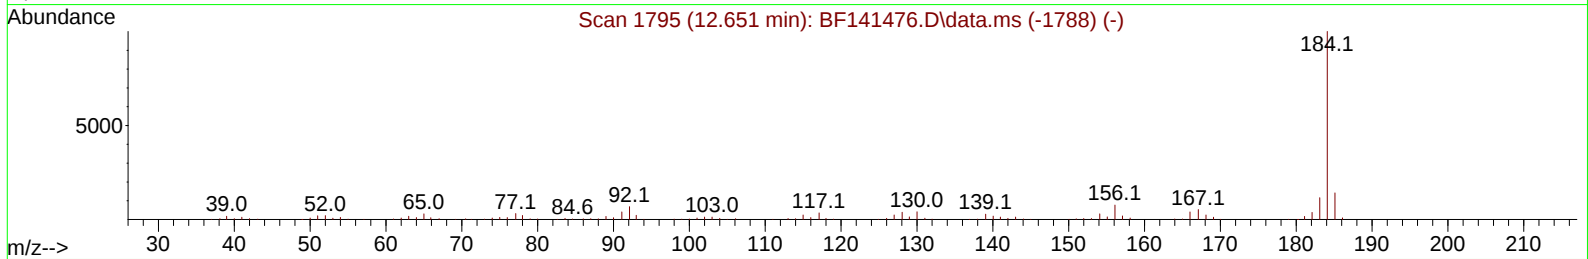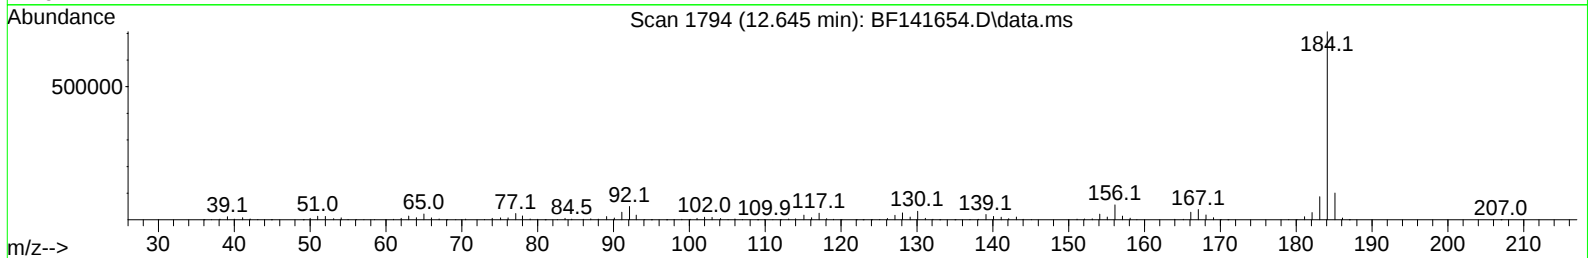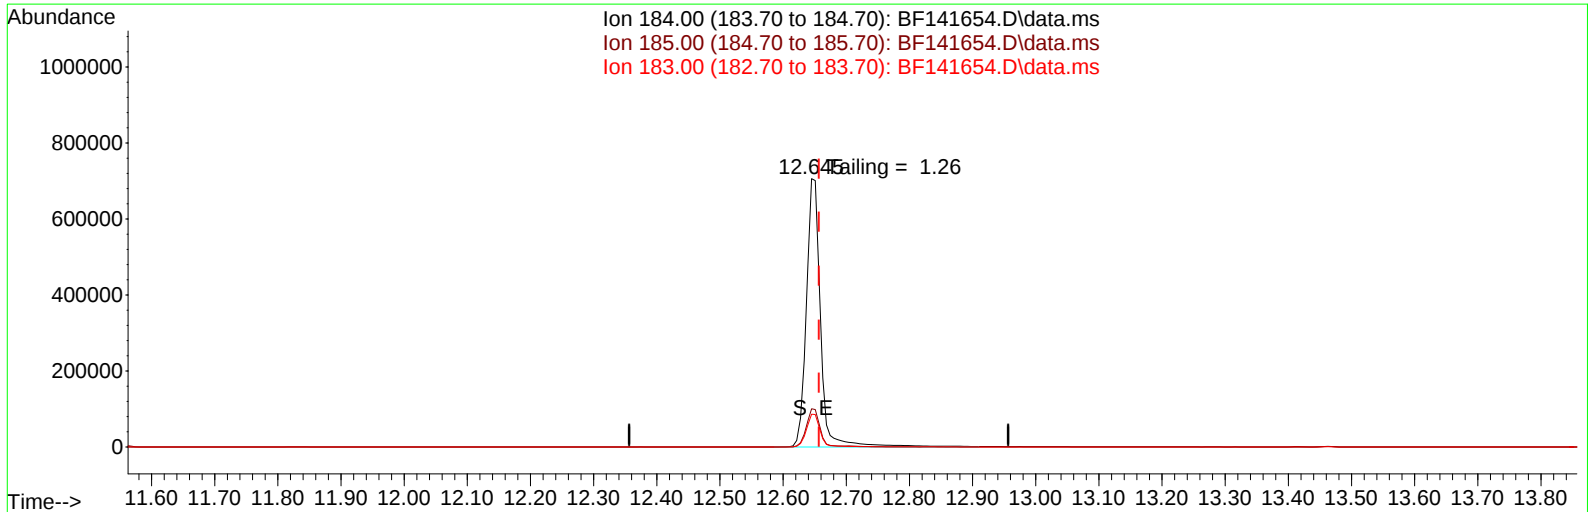

TIC: BF141654.D\data.ms

(77) Benzidine

12.645min (-0.012) 15778.91 ng

response 1110447

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.26
183.00	11.60	12.24
0.00	0.00	0.00