


Data Path : Z:\HPCHEM1\BNA_F\DATA\BF021915\
 Data File : BF077369.D
 Acq On : 19 Feb 2015 12:08
 Operator : TP/IZ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF021915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Feb 19 16:57:32 2015

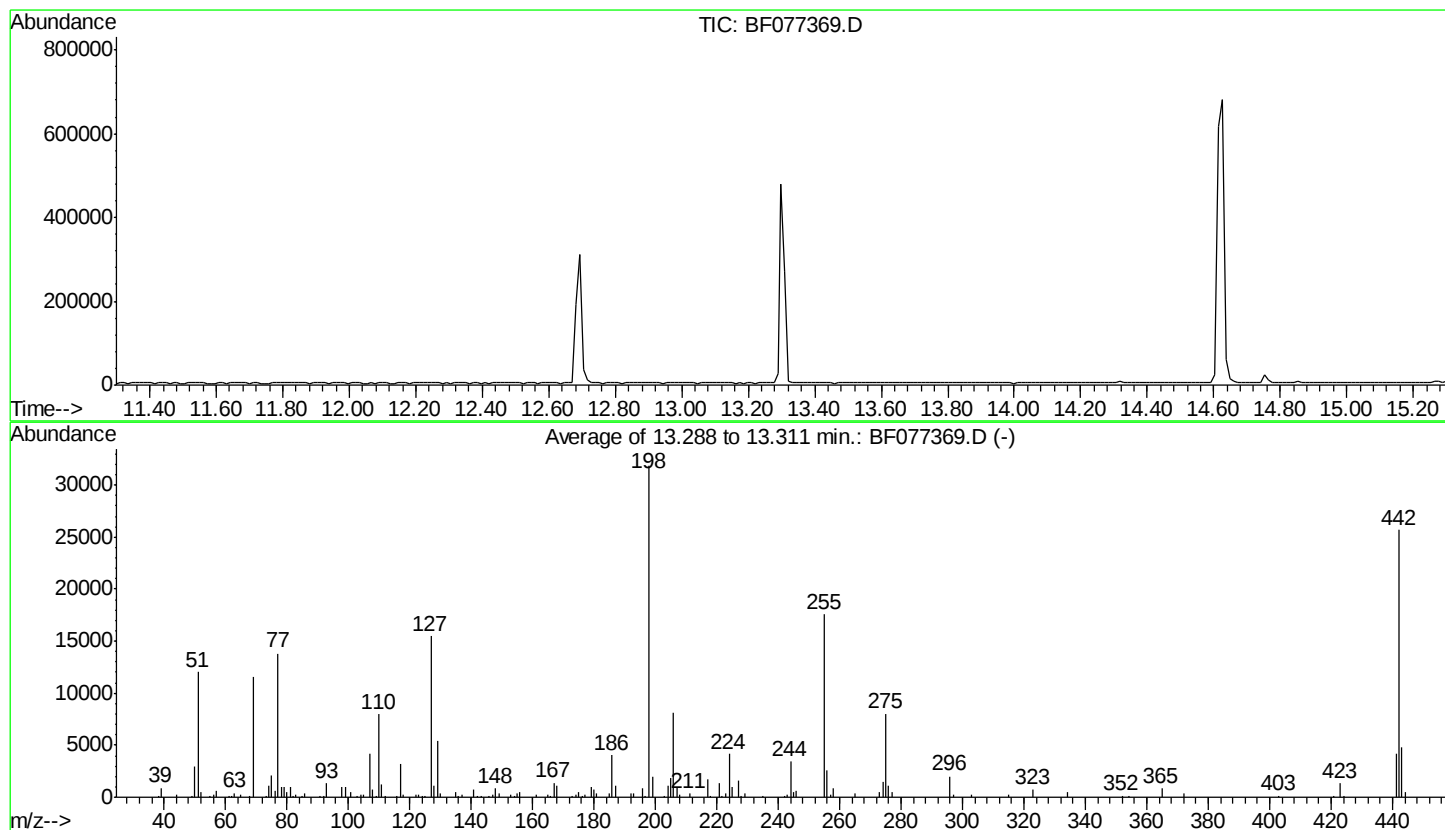

AutoFind: Scans 1085, 1086, 1087; Background Corrected with Scan 1082

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.7	12025	PASS
68	69	0.00	2	1.5	172	PASS
69	198	0.00	100	36.1	11513	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	48.6	15497	PASS
197	198	0.00	2	0.3	104	PASS
198	198	100	100	100.0	31861	PASS
199	198	5	9	6.2	1985	PASS
275	198	10	60	25.2	8040	PASS
365	198	1	100	2.6	824	PASS
441	442	0.01	24	16.2	4167	PASS
442	198	50	100	80.6	25666	PASS
443	442	15	24	18.9	4844	PASS