
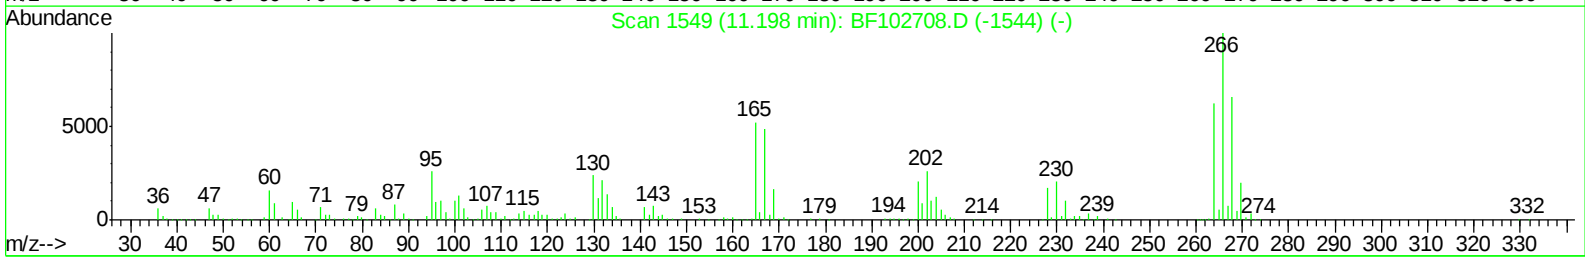
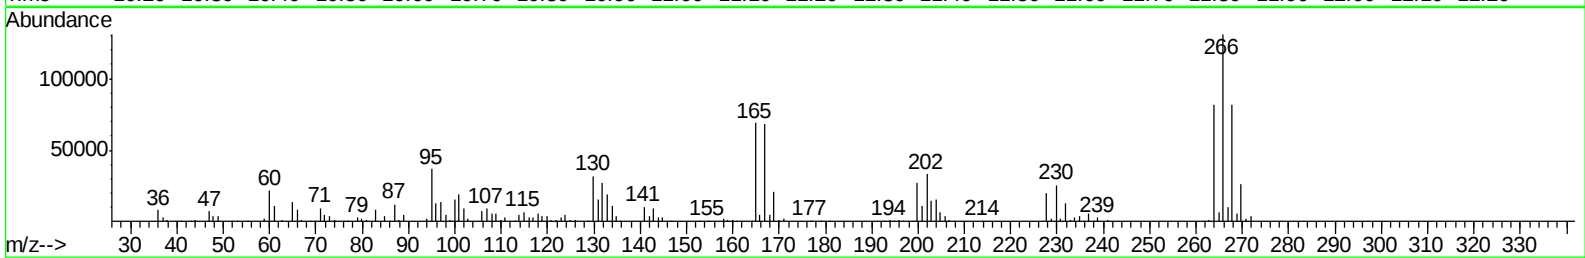


Data Path : Z:\HPCHEM1\BNA F\DATA\BF021918\
Data File : BF103068.D
Acq On : 19 Feb 2018 8:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 05:53:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 16 14:34:49 2018
Response via : Initial Calibration

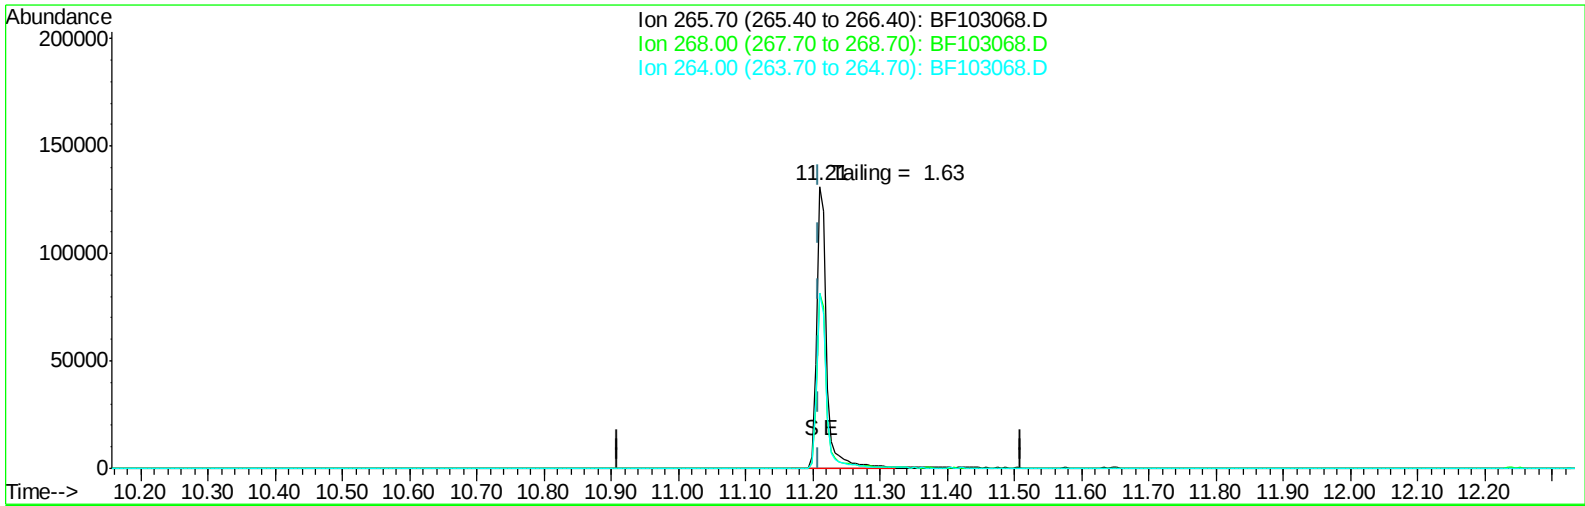

TIC: BF103068.D

(69) Pentachlorophenol (C)




11.210min (+0.000) 35120.28ng

response 138577

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.38
264.00	61.90	62.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA F\DATA\BF021918\
Data File : BF103068.D
Acq On : 19 Feb 2018 8:55
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 20 05:53:12 2018
Quant Method : Z:\HPCHEM1\BNA F\METHODS\8270-BF020318.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 16 14:34:49 2018
Response via : Initial Calibration

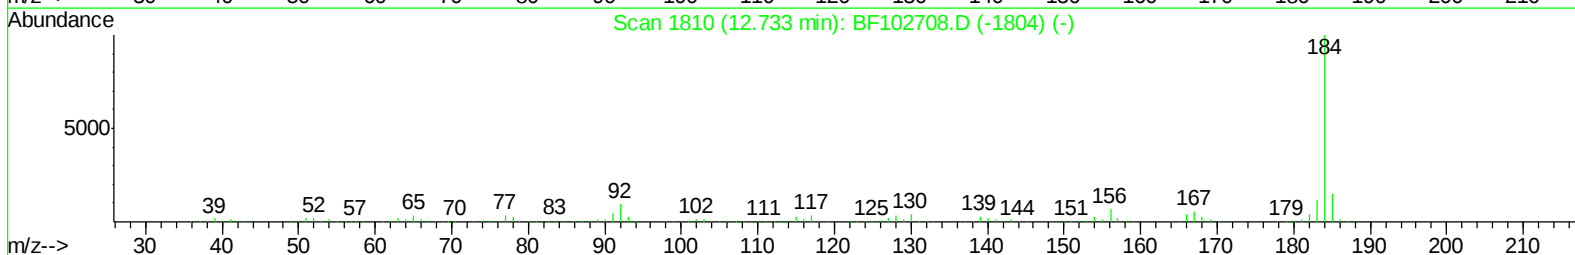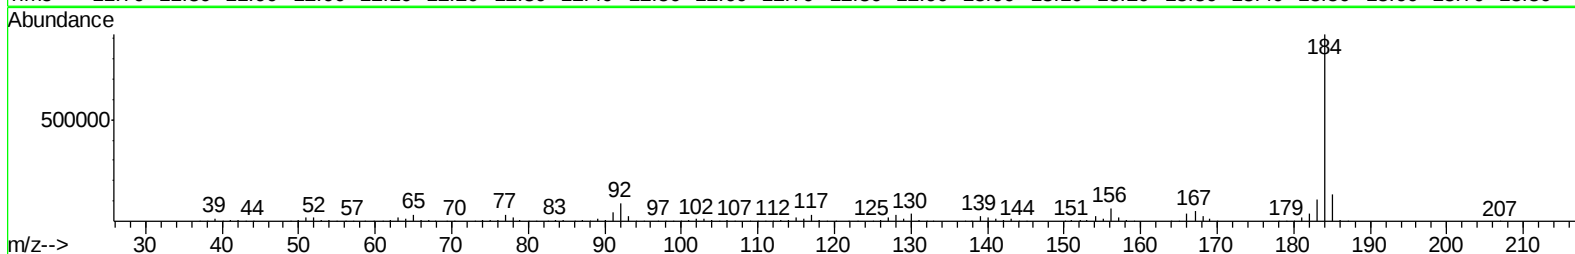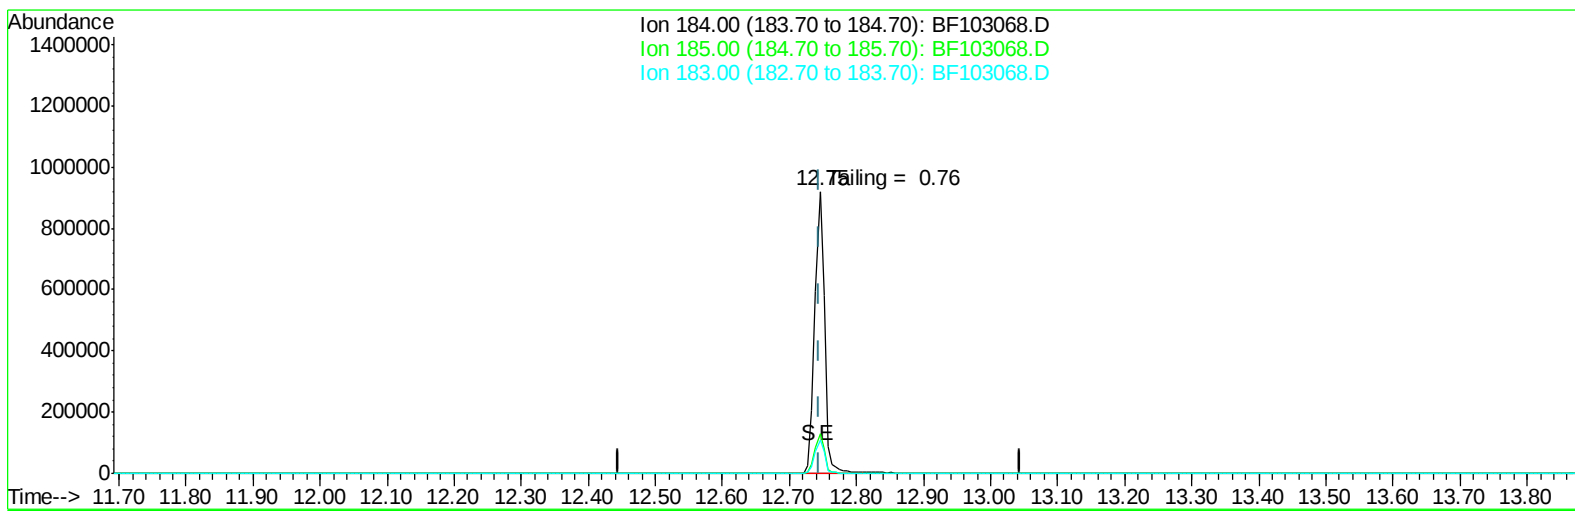

TIC: BF103068.D

(76) Benzidine

12.745min (+0.000) 169603.96ng

response 873044

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.33
183.00	11.60	12.04
0.00	0.00	0.00