


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF021918\
 Data File : BF103068.D
 Acq On : 19 Feb 2018 8:55
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 14:34:49 2018

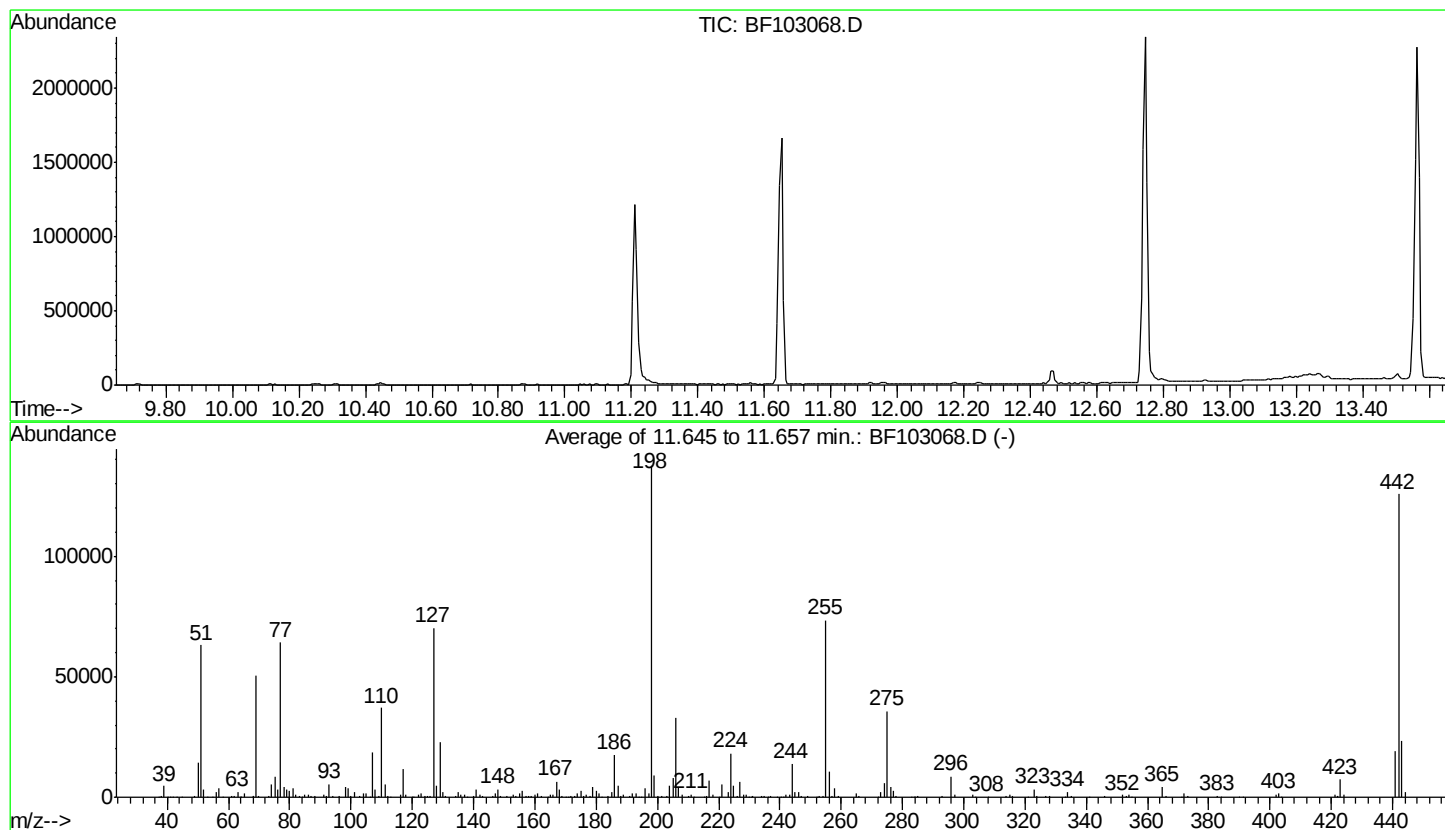

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1620

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.9	63102	PASS
68	69	0.00	2	0.8	416	PASS
69	198	0.00	100	36.9	50719	PASS
70	69	0.00	2	0.6	300	PASS
127	198	10	80	51.0	70213	PASS
197	198	0.00	2	1.1	1558	PASS
198	198	100	100	100.0	137605	PASS
199	198	5	9	6.5	8926	PASS
275	198	10	60	26.0	35720	PASS
365	198	1	100	3.3	4532	PASS
441	443	0.01	100	81.9	19268	PASS
442	198	50	100	91.5	125890	PASS
443	442	15	24	18.7	23514	PASS