


Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA_F\DATA\BF021918\
 Data File : BF103095.D
 Acq On : 19 Feb 2018 21:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_F\METHODS\8270-BF020318.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 16 14:34:49 2018

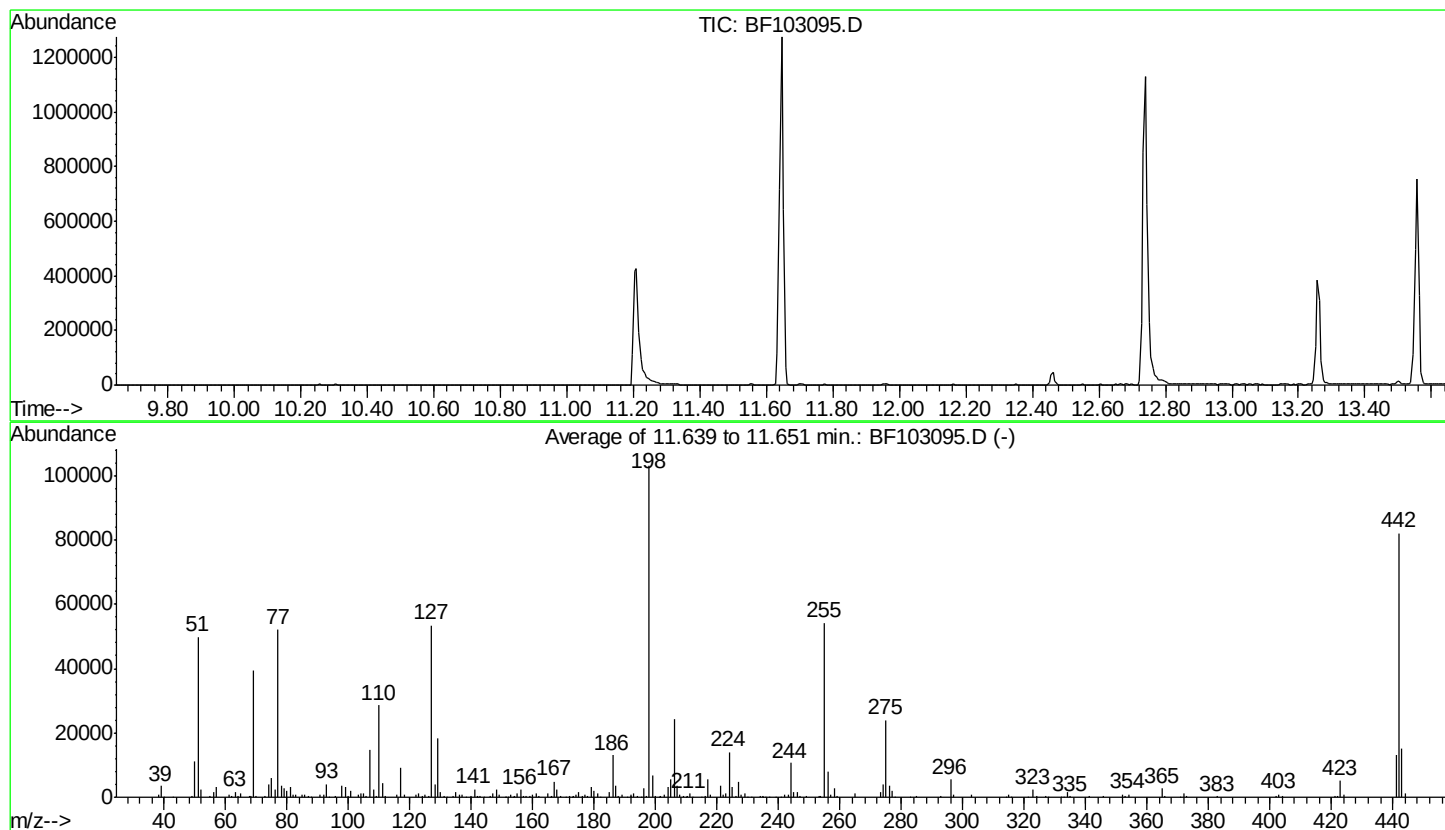

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.3	49744	PASS
68	69	0.00	2	0.9	336	PASS
69	198	0.00	100	38.2	39344	PASS
70	69	0.00	2	0.6	235	PASS
127	198	10	80	51.9	53506	PASS
197	198	0.00	2	0.4	395	PASS
198	198	100	100	100.0	103080	PASS
199	198	5	9	6.7	6908	PASS
275	198	10	60	23.2	23934	PASS
365	198	1	100	2.6	2696	PASS
441	443	0.01	100	86.2	13117	PASS
442	198	50	100	79.7	82181	PASS
443	442	15	24	18.5	15209	PASS