
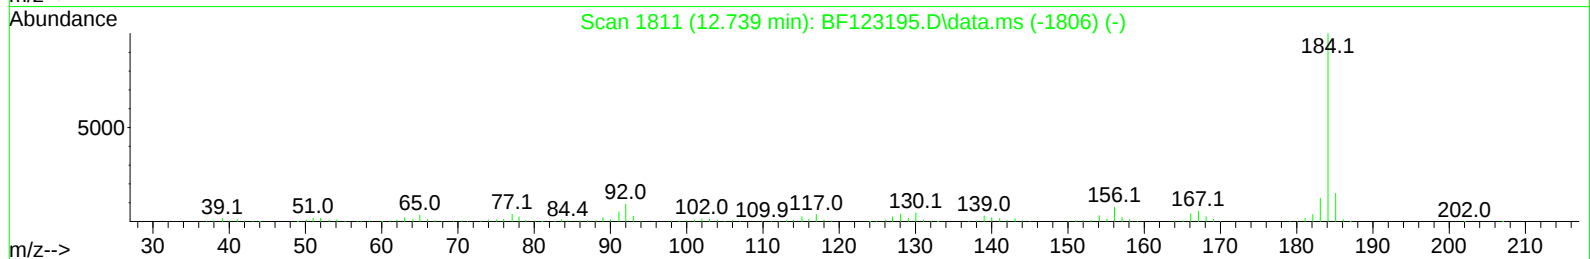
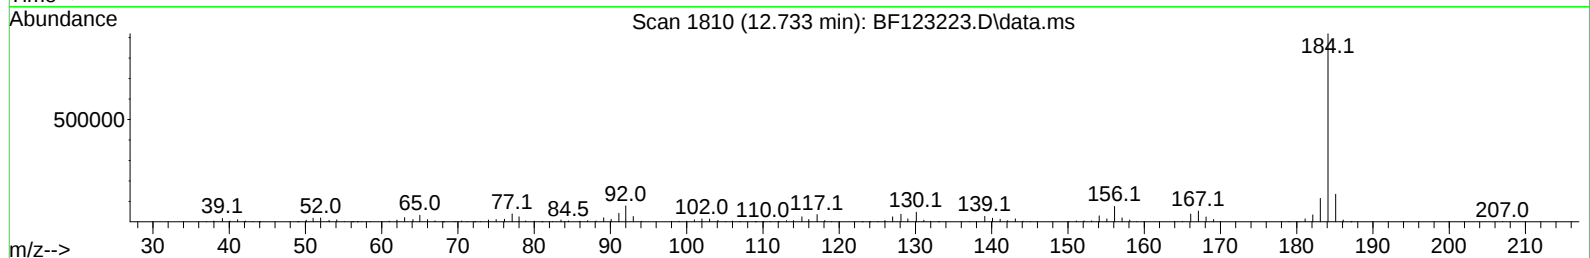


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123223.D
Acq On : 19 Feb 2021 10:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 11:38:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 11:33:56 2021
Response via : Initial Calibration

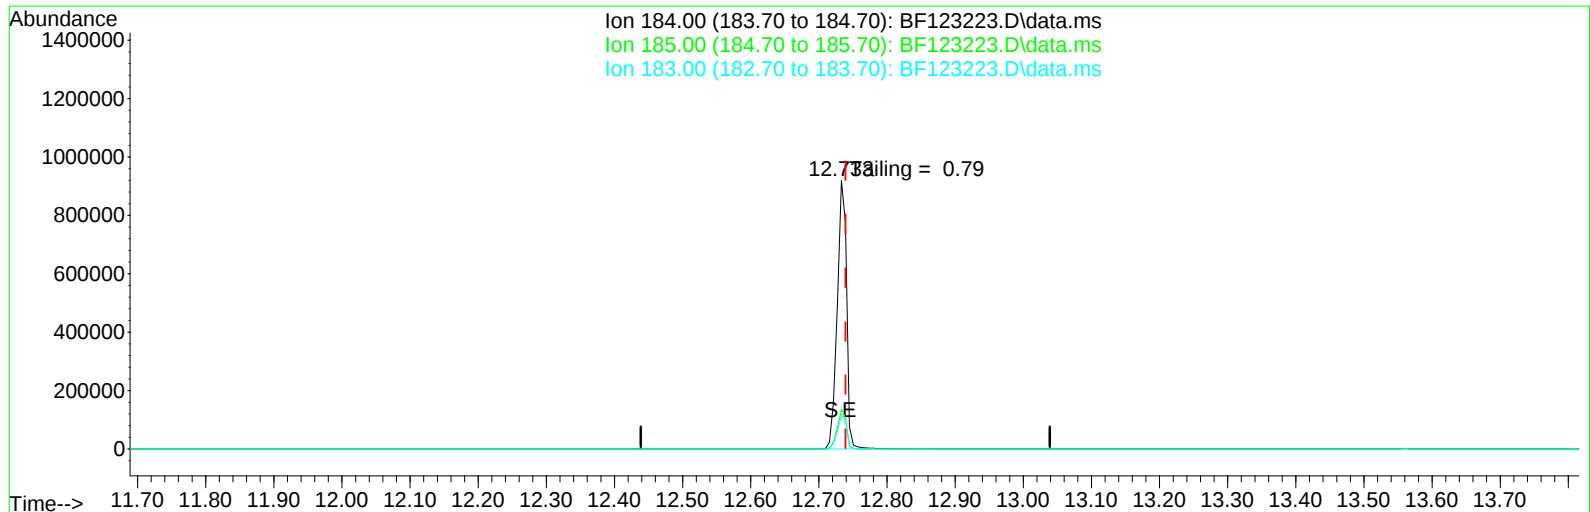

TIC: BF123223.D\data.ms

(77) Benzidine




12.733min (-0.006) 0.00 ng

response 880478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	12.10	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123223.D
Acq On : 19 Feb 2021 10:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 19 11:38:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 11:33:56 2021
Response via : Initial Calibration

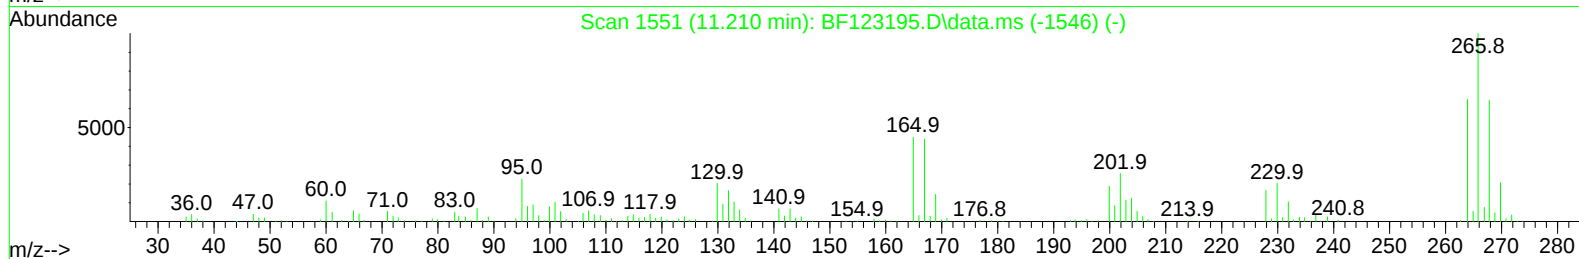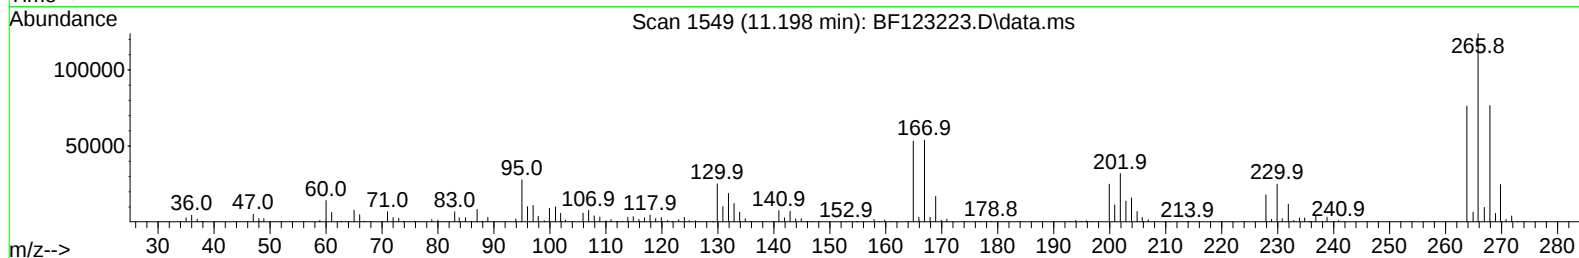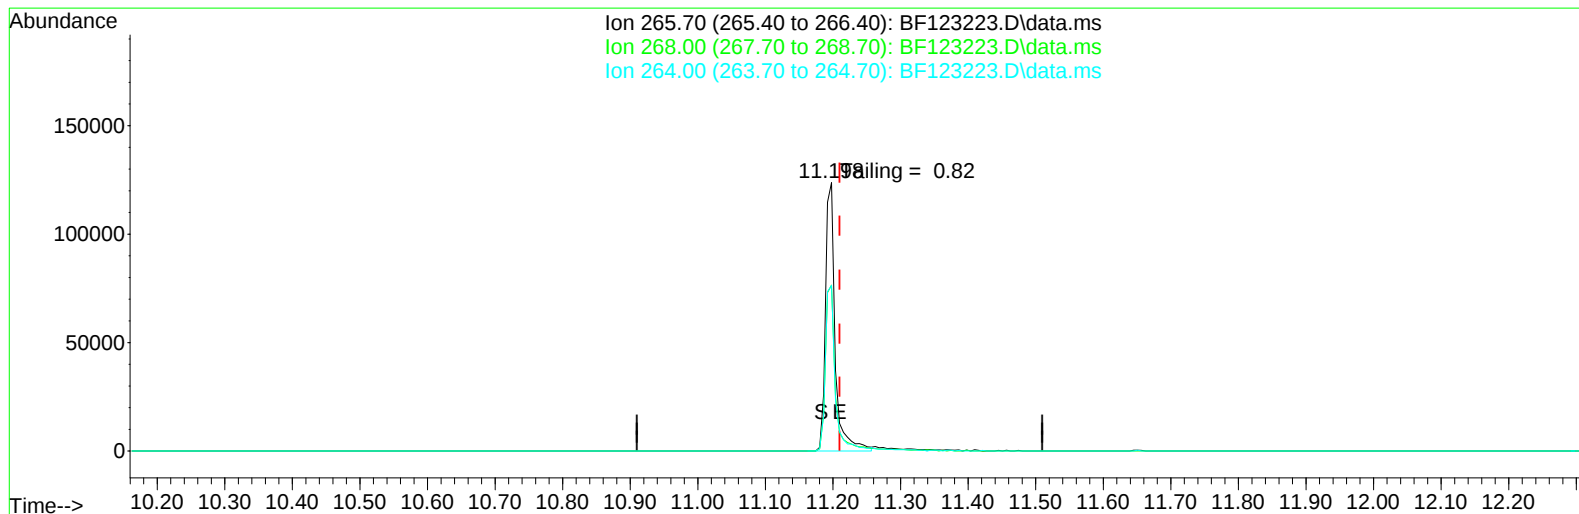

TIC: BF123223.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.012) 25810.39 ng

response 126976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.86
264.00	62.30	61.65
0.00	0.00	0.00