

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
 Data File : BF123232.D
 Acq On : 19 Feb 2021 18:18
 Operator : JU/CG
 Sample : PB134739BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB134739BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF123232.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.116	511	515	523	rVB	65708	93603	1.39%	0.224%
2	5.487	573	578	581	rBV	5771632	6306201	93.46%	15.075%
3	6.487	742	748	751	rBV	5255971	6303830	93.43%	15.070%
4	6.857	807	811	814	rBV	1526407	1262515	18.71%	3.018%
5	7.422	901	907	910	rBV	3727354	4172784	61.84%	9.975%
6	8.139	1024	1029	1033	rBV	1813279	1669580	24.74%	3.991%
7	9.222	1206	1213	1216	rBV	5357408	5673389	84.08%	13.563%
8	9.898	1322	1328	1332	rBV	1683183	1522823	22.57%	3.640%
9	10.692	1457	1463	1466	rBV	3290729	3168238	46.95%	7.574%
10	11.392	1575	1582	1585	rBV	1697796	1638612	24.29%	3.917%
11	12.986	1846	1853	1856	rBV	5928787	6747399	100.00%	16.130%
12	14.039	2028	2032	2035	rBV	1855496	1577881	23.39%	3.772%
13	15.515	2277	2283	2287	rBV	1276273	1555188	23.05%	3.718%
14	15.986	2356	2363	2367	rBV2	44572	70959	1.05%	0.170%
15	16.498	2445	2450	2457	rVB2	39980	67914	1.01%	0.162%




Sum of corrected areas: 41830916

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123232.D
Acq On : 19 Feb 2021 18:18
Operator : JU/CG
Sample : PB134739BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134739BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

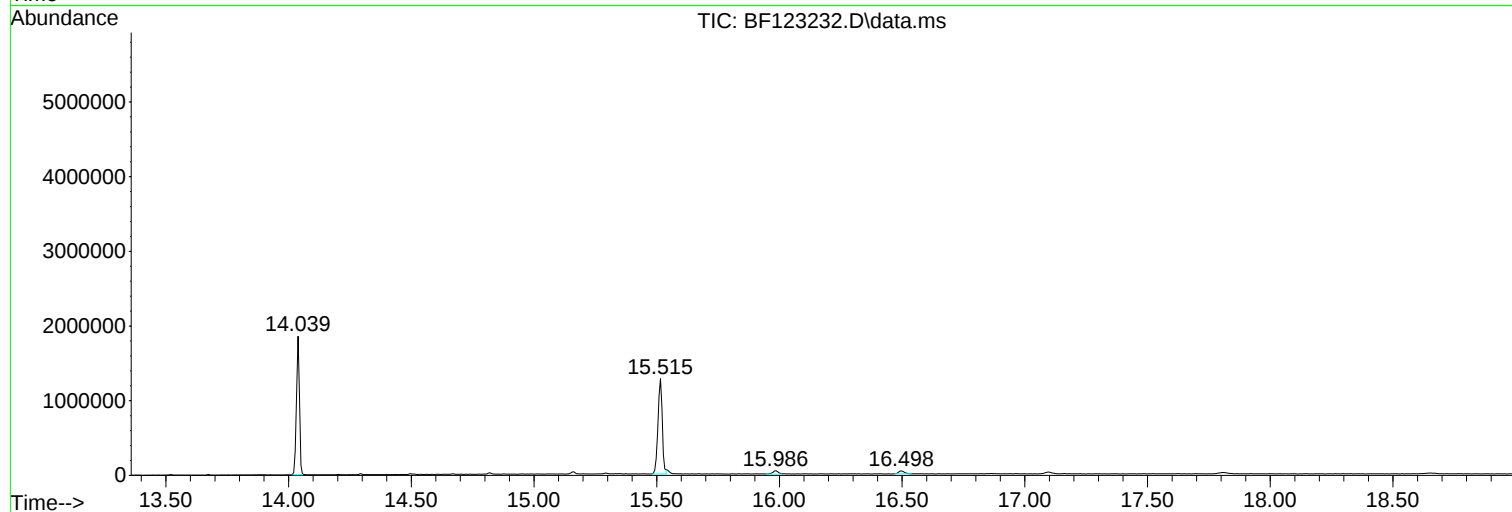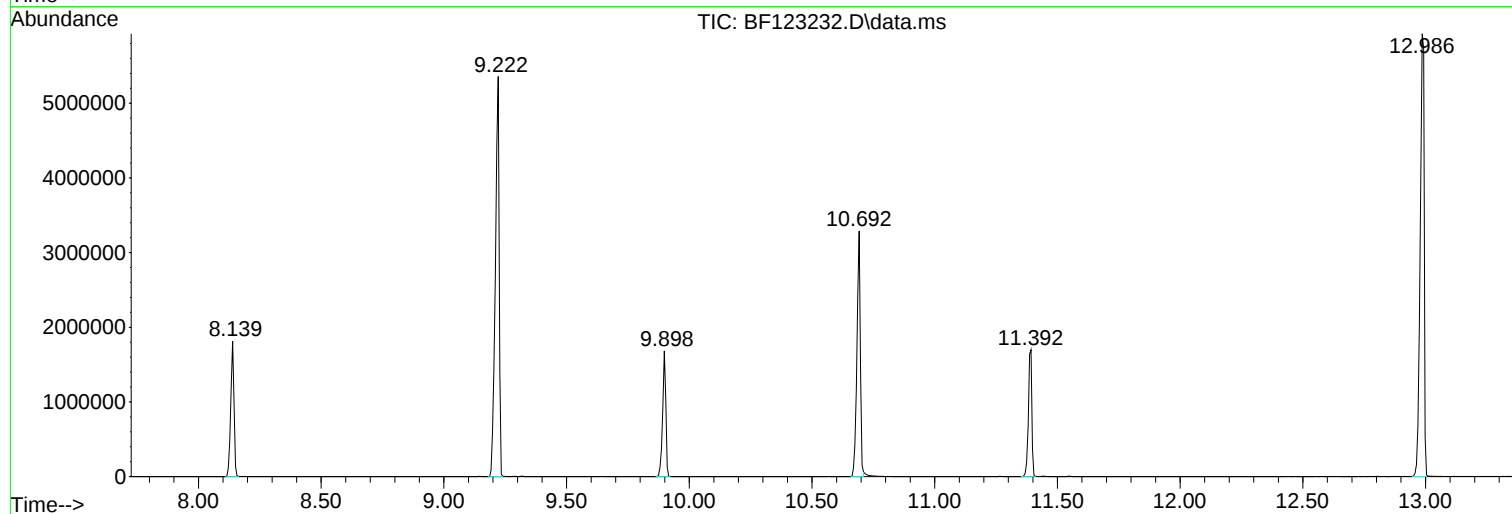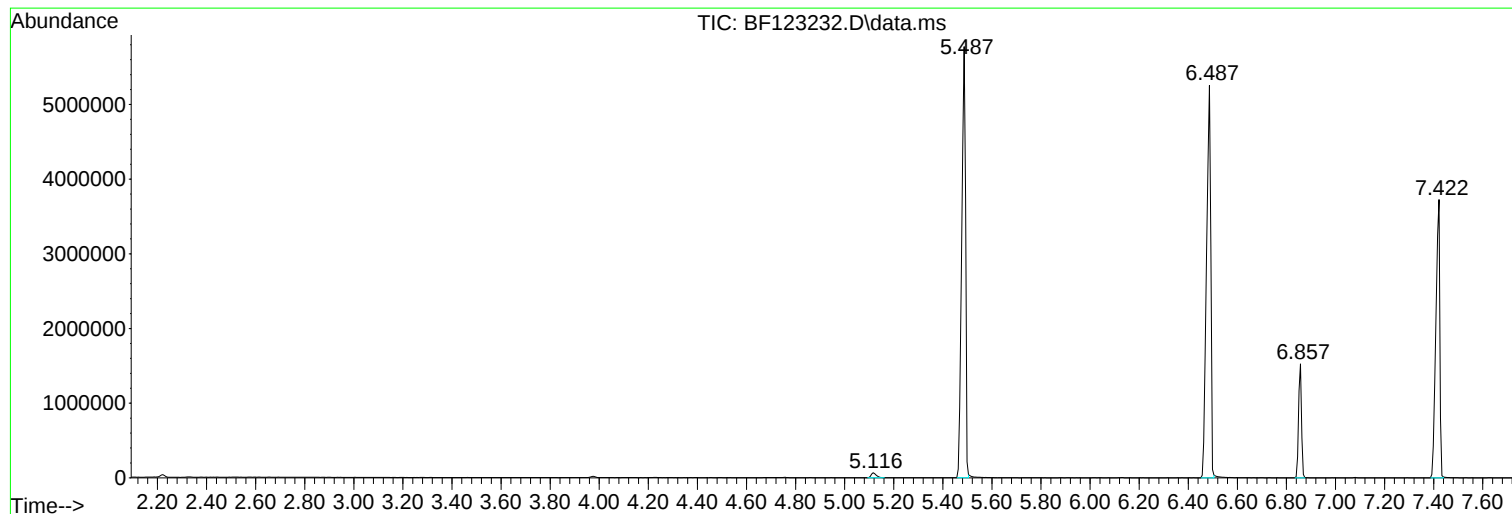

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123232.D
Acq On : 19 Feb 2021 18:18
Operator : JU/CG
Sample : PB134739BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134739BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123232.D
Acq On : 19 Feb 2021 18:18
Operator : JU/CG
Sample : PB134739BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB134739BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------