
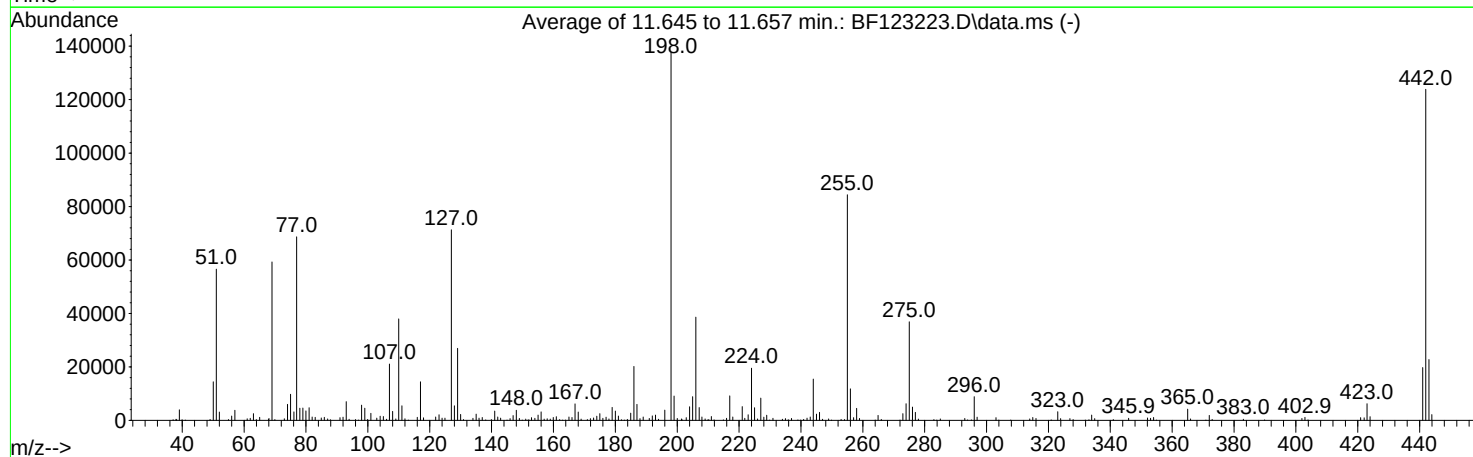


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
 Data File : BF123223.D
 Acq On : 19 Feb 2021 10:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 19 16:08:53 2021

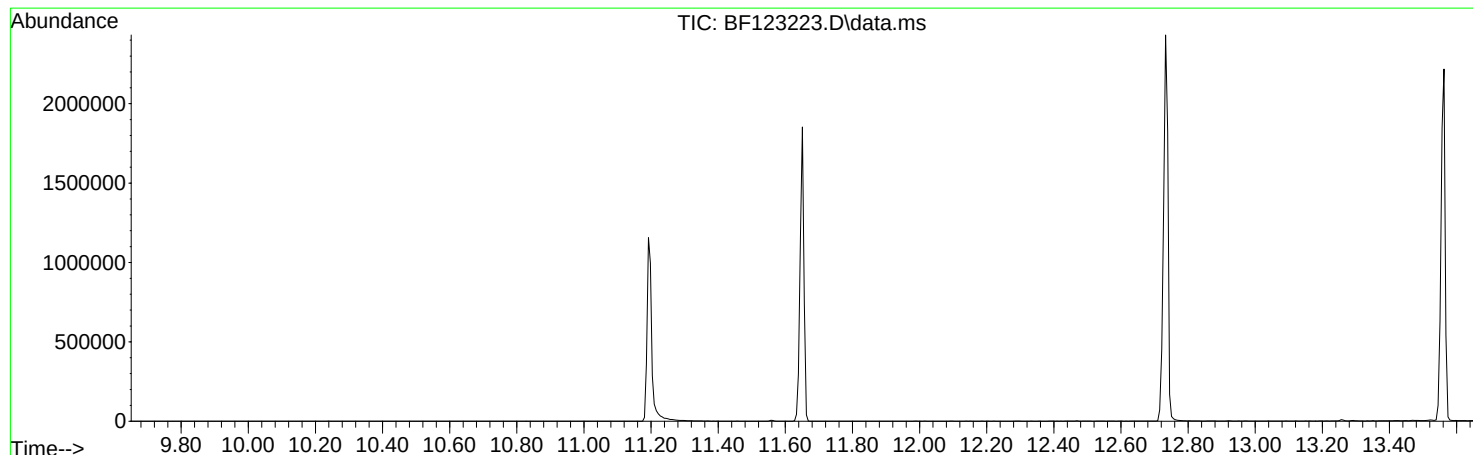




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	56560	PASS
68	69	0.00	2	1.3	742	PASS
69	198	0.00	100	43.1	59293	PASS
70	69	0.00	2	0.5	295	PASS
127	198	10	80	51.8	71331	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	137632	PASS
199	198	5	9	6.6	9073	PASS
275	198	10	60	26.8	36859	PASS
365	198	1	100	3.1	4207	PASS
441	198	0.01	100	14.4	19786	PASS
442	442	50	100	100.0	123835	PASS
443	442	15	24	18.4	22762	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
 Data File : BF123223.D
 Acq On : 19 Feb 2021 10:37
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Feb 19 11:38:50 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 19 11:33:56 2021
 Response via : Initial Calibration

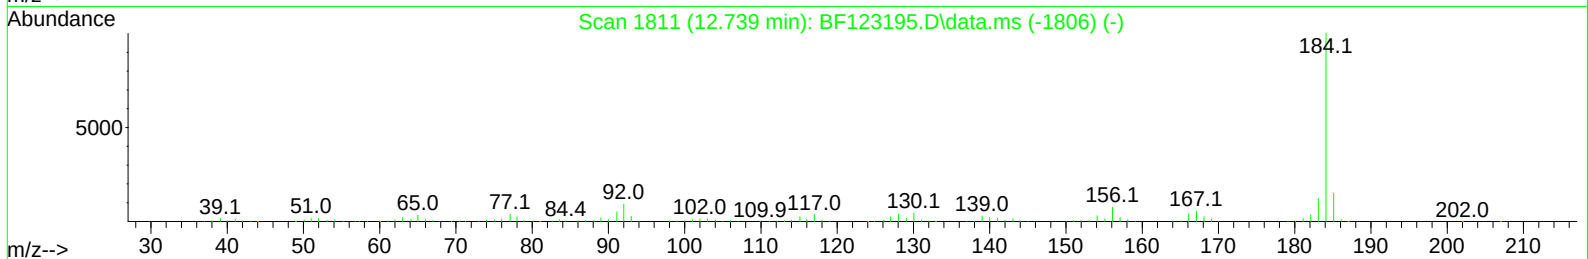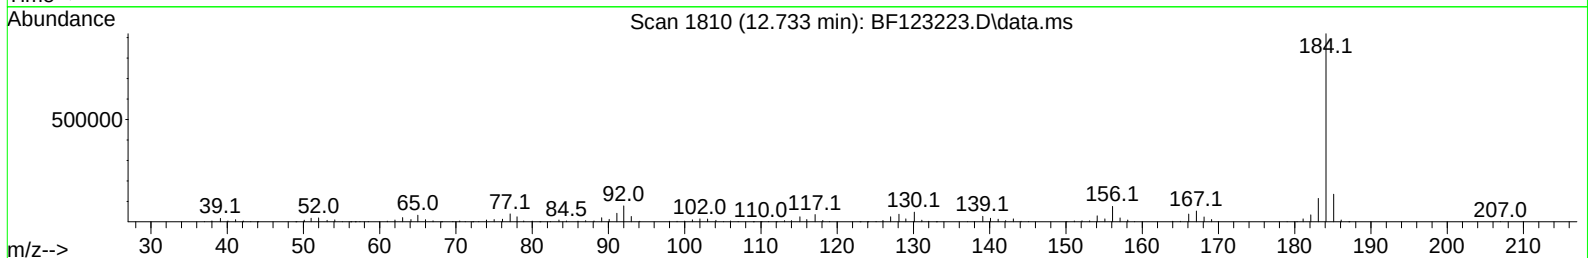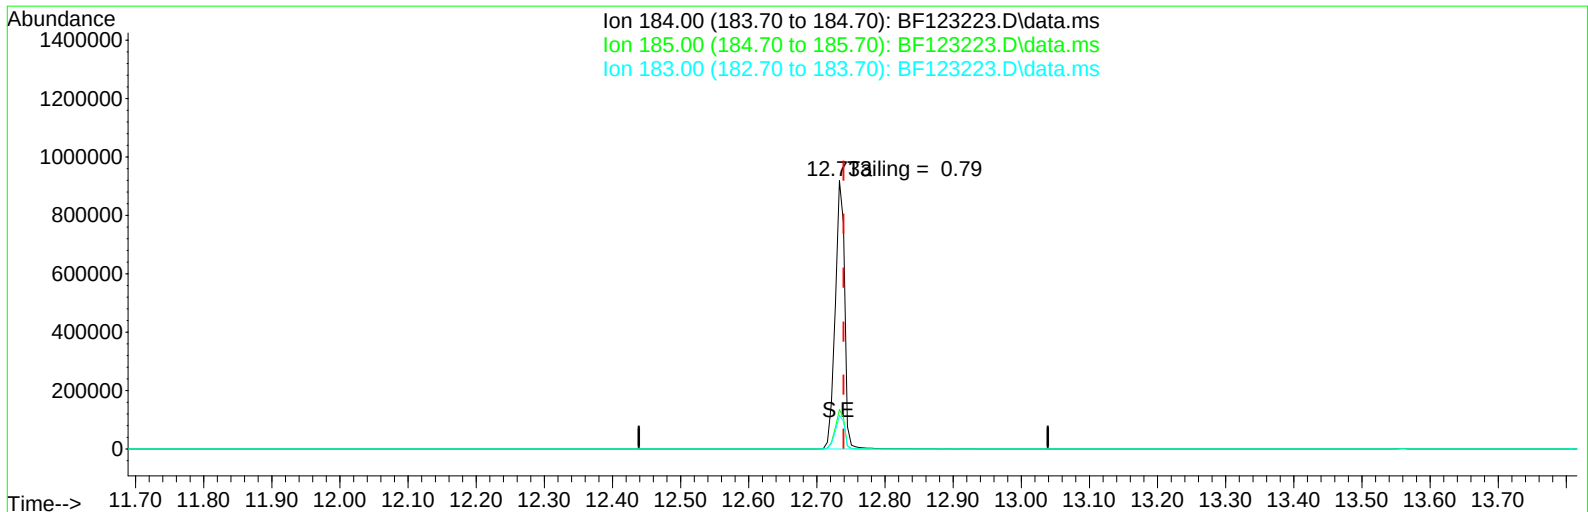

TIC: BF123223.D\data.ms

(77) Benzidine

12.733min (-0.006) 0.00 ng




response 880478

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.68
183.00	12.10	12.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021921\
Data File : BF123223.D
Acq On : 19 Feb 2021 10:37
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Feb 19 11:38:50 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF021921.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 19 11:33:56 2021
Response via : Initial Calibration

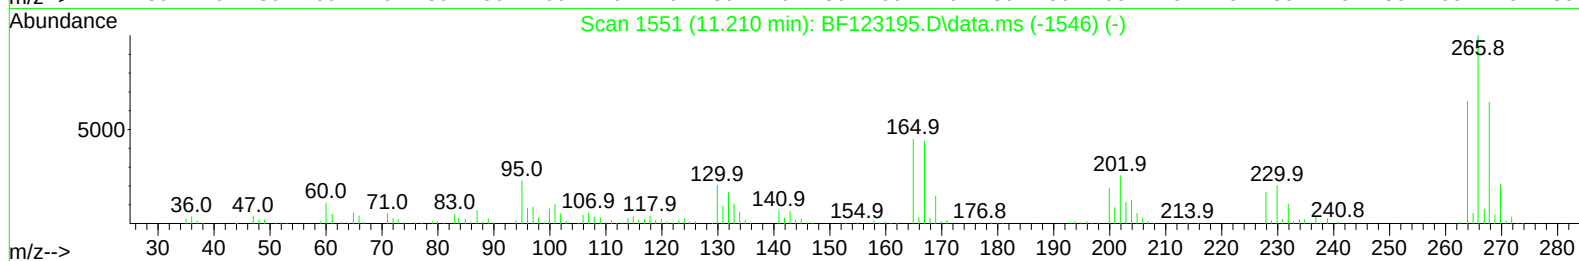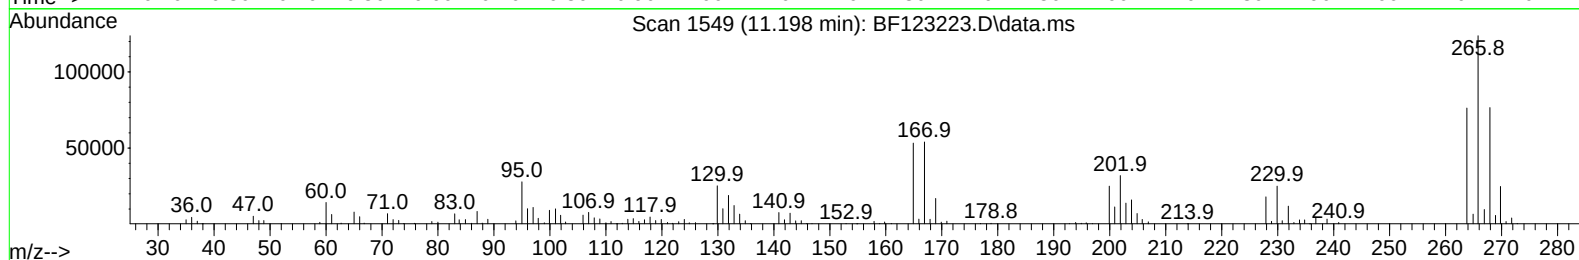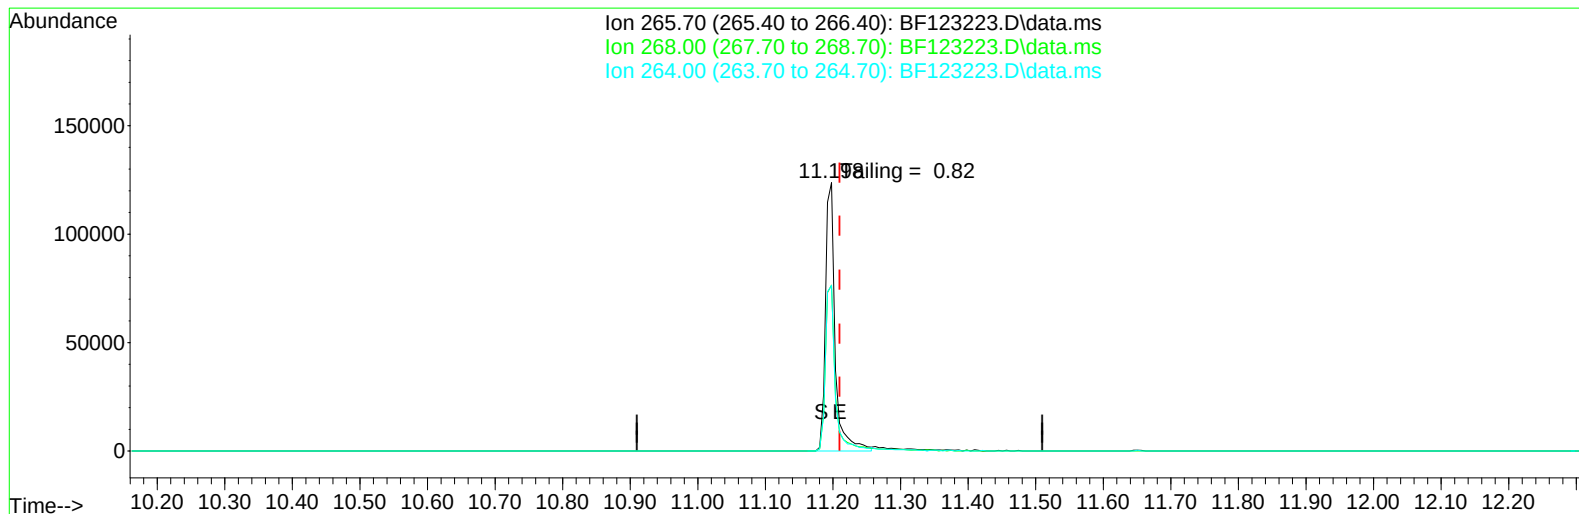

TIC: BF123223.D\data.ms

(70) Pentachlorophenol (C)

11.198min (-0.012) 25810.39 ng

response 126976

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	61.86
264.00	62.30	61.65
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_F
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
02/19/2021	BNA_F	<u>BF123223.D</u>
Compound Name	Response	Retention Time
DDT	348489	13.56
DDD	1962	13.25
DDE	504	12.92
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2466	350955	0.70