

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
 Data File : BF141674.D
 Acq On : 19 Feb 2025 14:46
 Operator : RC/JU
 Sample : Q1382-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OU4-PCS-TC-01-021725

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF141674.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.993	489	493	505	rVB	21048	35415	1.37%	0.188%
2	5.404	557	563	583	rBV	1513861	2084645	80.79%	11.064%
3	6.422	730	736	765	rBV	1513925	2163624	83.85%	11.483%
4	6.781	791	797	804	rBV	441191	562723	21.81%	2.987%
5	7.345	886	893	903	rBV	977845	1371757	53.16%	7.281%
6	7.604	929	937	949	rBV	34759	56706	2.20%	0.301%
7	8.063	1009	1015	1033	rBV	547004	753151	29.19%	3.997%
8	8.287	1048	1053	1061	rBV	18163	26733	1.04%	0.142%
9	9.134	1191	1197	1207	rBV	1929458	2552156	98.91%	13.545%
10	9.810	1307	1312	1325	rBV	635485	850124	32.95%	4.512%
11	10.022	1342	1348	1360	rBV5	13863	36835	1.43%	0.196%
12	10.528	1429	1434	1441	rVB	146529	190256	7.37%	1.010%
13	10.604	1441	1447	1463	rBV	1196708	1587696	61.53%	8.427%
14	11.298	1560	1565	1572	rBV	658644	839052	32.52%	4.453%
15	11.828	1648	1655	1668	rBV	477523	864621	33.51%	4.589%
16	12.539	1769	1776	1780	rBV8	9419	26080	1.01%	0.138%
17	12.610	1783	1788	1800	rBV	127599	263526	10.21%	1.399%
18	12.880	1829	1834	1846	rVB	1901940	2580229	100.00%	13.694%
19	13.557	1944	1949	1956	rVB	48302	89607	3.47%	0.476%
20	13.792	1983	1989	1994	rBV6	17795	46513	1.80%	0.247%
21	13.933	2008	2013	2023	rVB	439392	614869	23.83%	3.263%
22	14.104	2036	2042	2049	rBV	75776	140164	5.43%	0.744%
23	14.398	2088	2092	2096	rBV	18196	29830	1.16%	0.158%
24	14.574	2116	2122	2130	rBV	77538	134152	5.20%	0.712%
25	15.051	2195	2203	2208	rBV	74923	159200	6.17%	0.845%
26	15.380	2253	2259	2278	rBV	286872	523999	20.31%	2.781%
27	15.586	2289	2294	2303	rVB	54540	101156	3.92%	0.537%
28	16.198	2392	2398	2410	rBV	38929	93521	3.62%	0.496%
29	16.910	2515	2519	2528	rVB4	26779	63072	2.44%	0.335%




Sum of corrected areas: 18841412

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141674.D
Acq On : 19 Feb 2025 14:46
Operator : RC/JU
Sample : Q1382-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-01-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

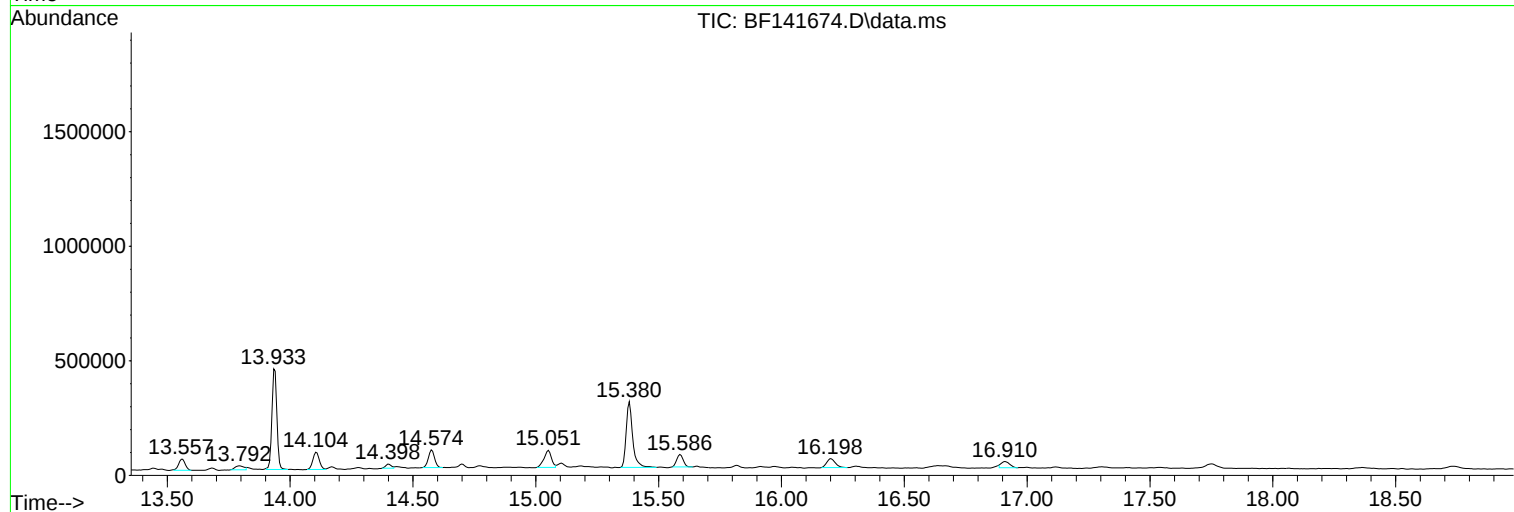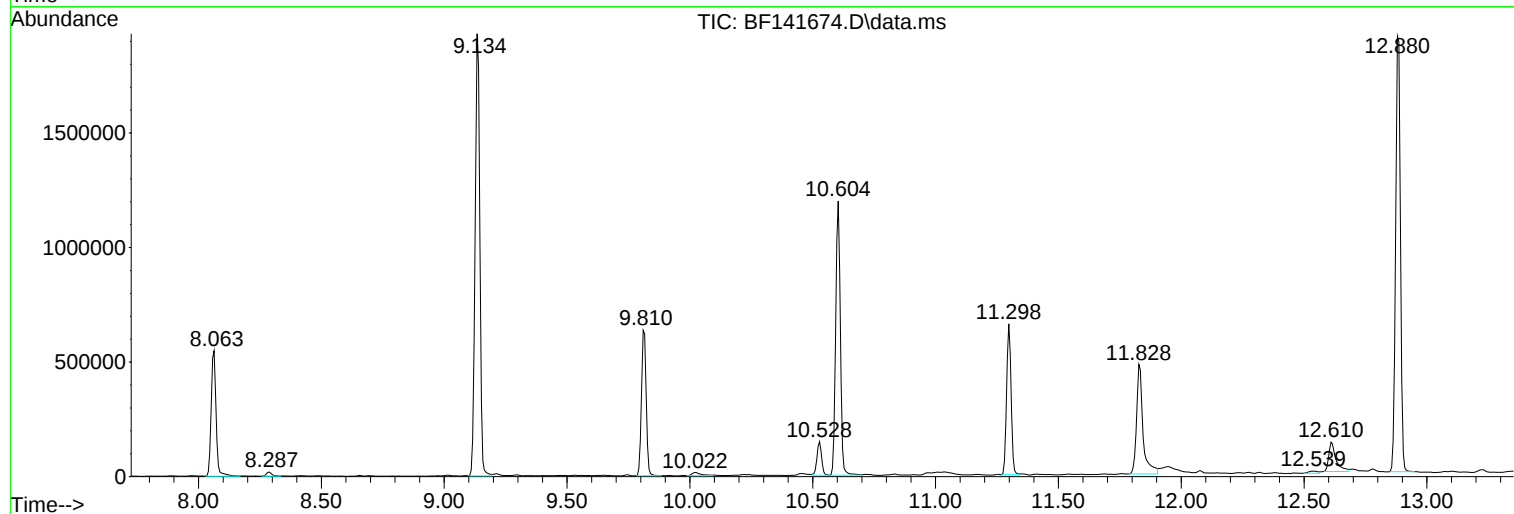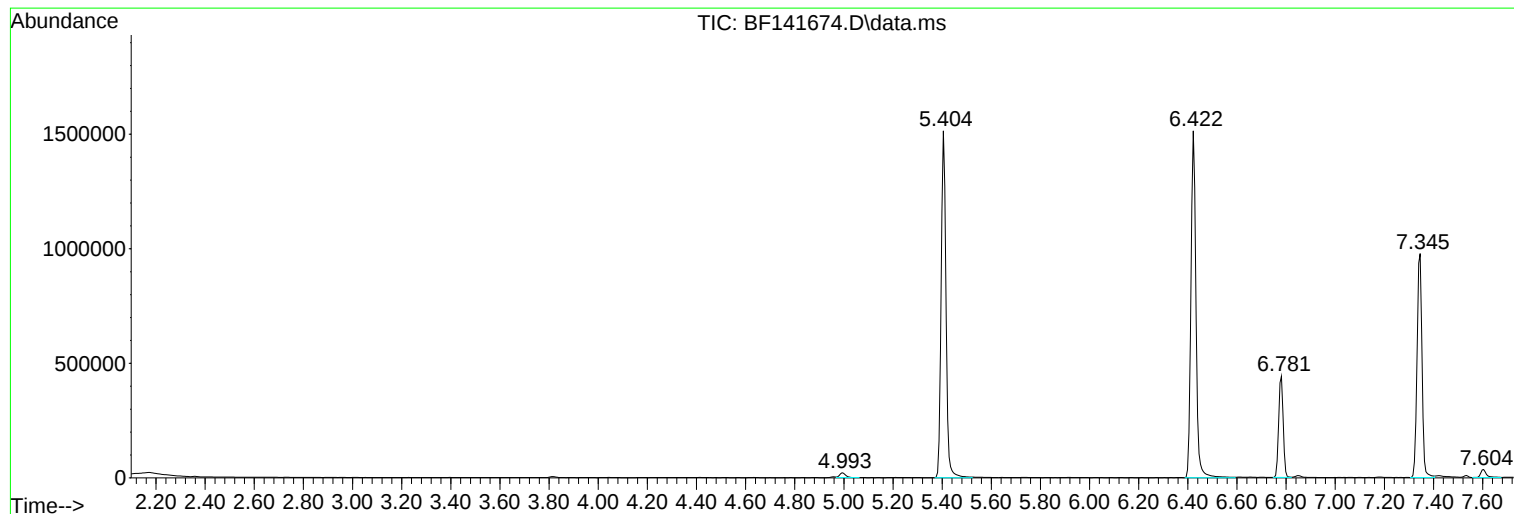

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141674.D
Acq On : 19 Feb 2025 14:46
Operator : RC/JU
Sample : Q1382-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-01-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF021925\
Data File : BF141674.D
Acq On : 19 Feb 2025 14:46
Operator : RC/JU
Sample : Q1382-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OU4-PCS-TC-01-021725

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF020625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------